WAVETEK

INSTRUCTION MANUAL

MODELS 158 AND 159 PROGRAMMABLE WAVEFORM GENERATORS

(Plus Option 159-005 Data)

INSTRUCTION MANUAL

MODELS 158 AND 159 PROGRAMMABLE WAVEFORM GENERATORS

(Plus Option 159-005 Data)

© - 1982 - Wavetek

THIS DOCUMENT CONTAINS INFORMATION PROPRIETARY TO WAVETEK AND IS SOLELY FOR INSTRUMENT OPERATION AND MAINTENANCE. THE INFORMATION IN THIS DOCUMENT MAY NOT BE DUPLICATED IN ANY MANNER WITHOUT THE PRIOR APPROVAL IN WRITING OF WAVETEK.

WAVETEK®

WAVETEK SAN DIEGO, INC.
9045 Balboa Ave., San Diego, CA 92123
P. O. Box 85265, San Diego, CA 92138
Tel 619/279-2200 TWX 910/335-2007

WAVETEK is a trademark of Wavetek Wandel Goltermann, Inc. (WWG) and is used by Fluke under a transitional license agreement. Fluke is not affiliated with WWG.

Manual Revision 8/83
Instrument Release U

WARRANTY

Wavetek warrants that all products of its own manufacture conform to Wavetek specifications and are free from defects in material and workmanship when used under normal operating conditions and within the service conditions for which they were furnished.

The obligation of Wavetek hereunder shall expire one (1) year after delivery and is limited to repairing, or at its option, replacing without charge, any such product which in Wavetek's sole opinion proves to be defective within the scope of this Warranty. In the event Wavetek is not able to repair or replace defective products or components within a reasonable time after receipt thereof, Buyer shall be credited for their value at the original purchase price.

Wavetek must be notified in writing of the defect or nonconformity within the warranty period and the affected product returned to Wavetek's factory or to an authorized service center within thirty (30) days after discovery of such defect or nonconformity. Shipment shall not be made without prior authorization by Wavetek.

This is Wavetek's sole warranty with respect to the products delivered hereunder. No statement, representation, agreement or understanding, oral or written, made by an agent, distributor, representative or employee of Wavetek, which is not contained in this warranty, will be binding upon Wavetek, unless made in writing and executed by an authorized Wavetek employee. **Wavetek makes no other warranty of any kind whatsoever, expressed or implied, and all implied warranties of merchantability and fitness for a particular use which exceed the aforestated obligation are hereby disclaimed by Wavetek and excluded from this agreement. Under no circumstances shall Wavetek be liable to Buyer, in contract or in tort, for any special, indirect, incidental or consequential damages, expenses, losses or delays however caused.**

CONTENTS

SECTION 1 INTRODUCTION

1.1 MODEL 158 1-1
1.2 MODEL 159 1-1
1.3. INTERFACE 1-1
1.4 OPTIONS 1-1
1.5 ACCESSORIES 1-1
1.6 PHYSICAL DESCRIPTION 1-1
1.7 SPECIFICATIONS 1-1

SECTION 2 INSTALLATION AND INTERFACE

2.1 MECHANICAL INSTALLATION 2-1
2.2 ELECTRICAL INSTALLATION 2-1

SECTION 3 OPERATION

3.1 INITIAL CHECKOUT 3-1
3.2 CONTROLS, INDICATORS AND PROGRAMMING 3-1
3.3 OPERATING PROCEDURE 3-3

SECTION 4 CIRCUIT DESCRIPTION

4.1 LOGIC NOTATION AND TERMINOLOGY 4-1
4.2 BASIC OPERATION 4-1
4.3 INPUT/OUTPUT 4-1
4.4 INTERFACE 4-1
4.5 KEYBOARD 4-1
4.6 DIGITAL BOARD CONTROL LOGIC 4-3
4.7 FREQUENCY D/A LOGIC 4-5
4.8 OFFSET D/A LOGIC 4-5
4.9 AMPLITUDE D/A LOGIC 4-5
4.10 DIGITAL BOARD DISPLAY (DRIVER) LOGIC 4-6
4.11 DISPLAY LOGIC 4-6
4.12 ANALOG BOARD 4-7

SECTION 5 CALIBRATION

SECTION 6 TROUBLESHOOTING

6.1 CORRECTIVE MAINTENANCE 6-1
6.2 TROUBLESHOOTING TECHNIQUES FOR INDIVIDUAL COMPONENTS 6-1

SECTION 7 PARTS LISTS AND SCHEMATIC DIAGRAMS

APPENDIX A GPIB, OPTION 005 . . . . . A-1

SAFETY

This instrument is wired for earth grounding via the facility power wiring. Do not bypass earth grounding with two wire extension cords, plug adapters, etc.

BEFORE PLUGGING IN the instrument, comply with installation instructions.

MAINTENANCE may require power on with the instrument covers removed. This should be done only by qualified personnel aware of the electrical hazards.

The instrument power receptacle is connected to the instrument safety earth terminal with a green/yellow wire. Do not alter this connection. (Reference: ⏚ or ⚠ stamped inside the rear panel near the safety earth terminal.)

WARNING notes call attention to possible injury or death hazards in subsequent operations.

CAUTION notes call attention to possible equipment damage in subsequent operations.

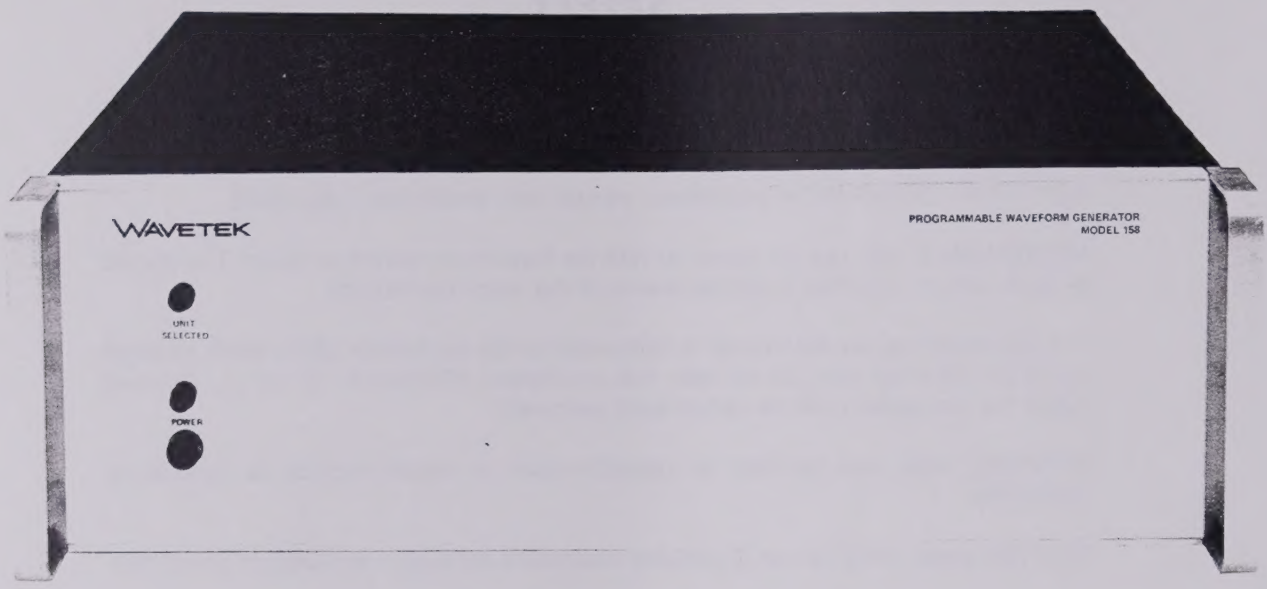

Wavetek Model 158 Programmable Waveform Generator

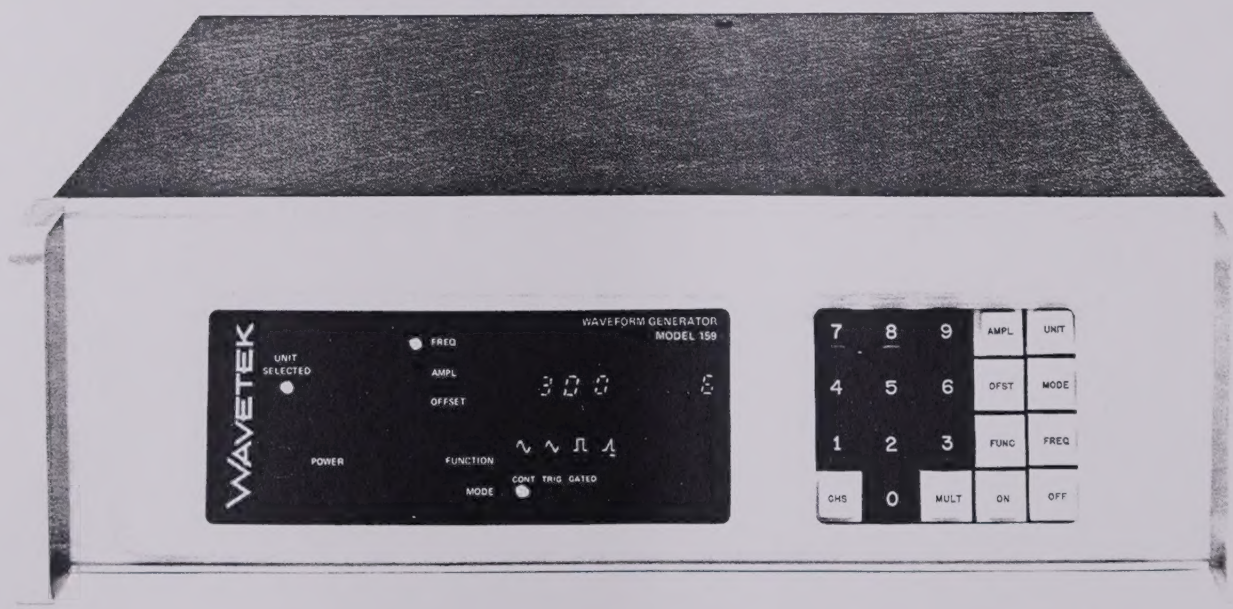

Wavetek Model 159 Programmable Waveform Generator

Figure i – Model 158 and 159 Programmable Waveform Generators

SECTION 1
INTRODUCTION

1.1 MODEL 158

The Wavetek Model 158 Waveform Generator is a remote-control only Model 159 generator (without front panel controls and indicators). All information on the Model 159 generator also pertains to the Model 158 generator except local operation.

1.2 MODEL 159

The Wavetek Model 159 Waveform Generator is digitally controlled locally with front panel, keyboard pushbuttons, and remotely with a selection of 21 ASCII (7-level) "typing" characters (with appropriate external interface). The effect of each control is digitally displayed on the front panel with red LED (light emitting diode) indicators. Numeric readout of frequency, offset and amplitude is in 3-digit scientific notation.

Sine, triangle, square, and ramp waveforms of frequencies from 1 Hz to 3 MHz and amplitudes from 10 mV p-p to 10V p-p can be generated. Waveform generation can be continuous, triggered for just one cycle at a time, or gated for as many cycles or for as long as desired. Waveform center reference levels can be offset positive or negative from 10 mV to 5V and waveform phase, or polarity, can be inverted (180 degrees).

Along with the main 50 ohm output at the rear panel, which is the controlled waveform signal output, the generator delivers a square wave of the selected frequency for a synchronizing pulse output.

Analog inputs are received at the rear panel for a triggering input for triggered and gated operations, and a voltage controlled generator (VCG) input for frequency proportional to input dc levels. The 50Ω OUT signal can be swept in a 1000:1 frequency ratio, frequency modulated or dc programmed by the VCG input. The trigger and gate modes can be used for pulse output, one cycle output or tone bursts.

Up to nine generators can be connected in parallel with one another as a multiple unit group. Each generator is internally configured with its own address, or unit select code, from 1 to 9. For example, an installation may have one master display and keyboard panel, which is used to address and command the slave generators. The status of the addressed generator would be displayed.

1.3 INTERFACE

The generator accepts TTL ground true 7-bit ASCII "typing" characters serially; the 7 bits of each character are accepted in parallel. A clock line in parallel with the data bits is used to clock in the data characters. Computer control is accepted as is keyboard control from another generator in multiple unit groups. With computer control, the generator keyboard control panel can be locked out, or disabled, to prevent control competition.

1.4 OPTIONS

Several interface options are available for the Model 158 and 159 generators. They include input isolation, RS232 and IEEE 488 compatible data converters.

1.5 ACCESSORIES

Accessories for the generators include interfaces for several mini-computers.

1.6 PHYSICAL DESCRIPTION

The mechanical characteristics of the Models 158 and 159 are given in Paragraph 1.7.8. The standard models come equipped with a 10 foot, 3 wire detachable power cord and rack mount adapters. Interface cabling requires Molex brand connectors (see Paragraph 2.2.3); one is furnished.

1.7 SPECIFICATIONS

1.7.1 Versatility

Waveforms

Sine ∿ , triangle ∧ , square ⎍ , ramp ◿ (50% duty cycle), and auxiliary TTL sync pulse. All selectable waveforms may be inverted.

Frequency Range

Sine, triangle, and square from 1 Hz to 3 MHz in 7 ranges with 3-digit resolution.

10^0	1 Hz to 9.99 Hz
10^1	10 Hz to 99.9 Hz
10^2	100 Hz to 999 Hz
10^3	1 kHz to 9.99 kHz
10^4	10 kHz to 99.9 kHz
10^5	100 kHz to 999 kHz
10^6	1 MHz to 3 MHz

Ramp from 1 Hz to 1 MHz in 6 ranges ($10^0 \longrightarrow 10^5$).

NOTE

Generator is usable from 0.01 Hz with derated accuracies.

Main Output

Three digits of amplitude from 10 mV to 10V p-p into 50Ω (20V p-p into an open circuit) in 3 ranges (10^0, 10^{-1}, 10^{-2}).

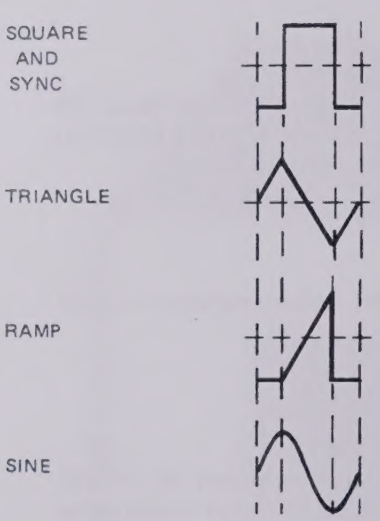

NORMAL PHASE RELATIONSHIPS

DC Offset

Three digits of dc offset to ±5V into 50Ω. DC offset plus waveform peak value may not exceed 10V peak into open circuit or 5V peak into 50Ω.

Sync Output

A TTL compatible 0 to 2.5V square wave output, which provides 50 mA sinking current to sync up to 30 TTL loads.

Data Entry

Front panel keyboard/display and remote programming (Model 159).
Remote programming only (Model 158).

1.7.2 Operational Modes

Continuous, triggered, and gated operation provided. In triggered mode, one cycle of selected signal output for each input trigger signal. In gated mode, signal output at selected frequency for duration of the input gate plus completion of the last cycle. Model 159 has front panel manual trigger.

Trigger/Gate Signal

Minimum	+2V
Maximum	50V
Input Impedance	1 kΩ

1.7.3 Analog Modulation Control

Frequency may be externally controlled by analog voltage (VCG) providing dc programming for FSK or wide band ac modulation. Input impedance is 5 kΩ.

VCG Control Signal

Approximately 2.5V	1000:1 frequency change
Approximately 7.5V	3000:1 frequency change
	(300% overrange in first 6 ranges)

VCG Small Signal Bandwidth

100 kHz

VCG Slew Rate

4% of range per μs

1.7.4 Accuracy

Horizontal Precision (Frequency Accuracy)

10 Hz to 100 kHz	±1% of program value ±1 digit
100 kHz to 1 MHz	±2% of program value ±1 digit
1 MHz to 3 MHz	±4% of program value ±1 digit

Vertical Precision (Amplitude Accuracy)

NOTE

Vertical precision stated is for 10^0 amplitude multiplier. For 10^{-1} and 10^{-2}, add 1% per step.

Vertical Precision (Amplitude Accuracy) (Continued)

Sine and Square Waveforms:
10 Hz to 100 kHz . . . ±2% of program value ±1 digit
100 kHz to 1 MHz . . . ±5% of program value ±1 digit

Triangle and Ramp Waveforms:
10 Hz to 10 kHz . . . . ±2% of program value ±1 digit

DC Offset

±2% of program value ±1 digit

Sine Wave Frequency Response

Amplitude change with frequency less than:
0.1 dB to 100 kHz
0.5 dB to 1 MHz
1.0 dB to 3 MHz

Stability

Short term . . . . . ±0.05% for 10 minutes
Long term . . . . . ±0.25% for 24 hours

1.7.5 Purity

Sine Wave Distortion

Total harmonic distortion less than:
0.5% to 30 kHz . . . . . ranges 10^0 thru 10^3
1.0% to 300 kHz . . . . . ranges 10^0 thru 10^4

All harmonics:
34 dB down to 1 MHz

Time Symmetry

1% to 100 kHz

Amplitude Symmetry

All waveforms to 100 kHz are symmetrical about ground within 1% of maximum p-p amplitude.

Triangle Linearity

Greater than 99% to 100 kHz

Square Wave Rise and Fall Time

Less than 50 ns

Total Aberrations

Less than 5% of program value ±20 mV

1.7.6 Programming

Programming Transition Time

Unit accepts bytes at a 1 MHz rate. The output will become stable within 100 μs unless the range digit is changed; then output will be stable within 1 ms.

Isolation

Signal ground and program ground are common in the standard 158/159. Optical isolation is available.

Logic Level Requirements

State	Requirements
Low (Logic "1")	0V to 0.4V sinking 25 mA maximum
High (Logic "0")	2.4V or open

NOTE

1. *Open input is 3.0V.*
2. *Input is terminated by 220Ω to +5V and 330Ω to ground.*
3. *Recommended driver: SN 7438.*

Input Control Lines and Connector Layout

Mating Connector: Molex 03-09-2151 with 02-09-2118 pins

J9 Pin No.	Designation	
13	XD0	Least significant bit
11	XD1	
8	XD2	
10	XD3	Input data lines
9	XD4	
12	XD5	
14	XD6	Most significant bit
15	XCLK	Clock control
7	Common	
3	Keyboard Enable	
1	Keyboard Enable Return	

Keyboard to ASCII Conversion Table

Keyboard	ASCII
AMPL	A
UNIT	G
OFST	D
MODE	B
FUNC	C
FREQ	F

Keyboard	ASCII
MULT	(Space) or E
ON	H
OFF	I
0 thru 9	0 thru 9
CHS	– (Minus)

Timing

Direct (No Isolation)

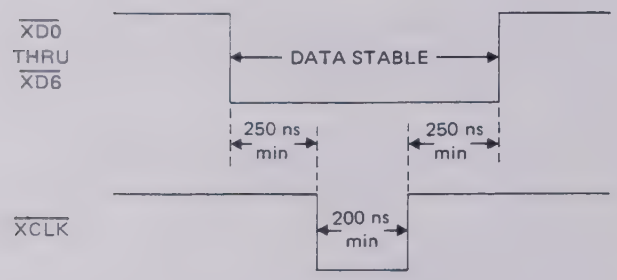

1.7.7 Environmental

Specifications apply for 25°C ±5°C. For operation from 0°C to +55°C, derate all specifications by a factor of 2. Unit may be stored from −40°C to +75°C without damage.

1.7.8 Mechanical

May be used on the bench or in a 19 inch rack. Rack adapter hardware and program mating connectors included.

Dimensions

17¼ in./43.8 cm wide, 5¼ in./13.3 cm high, 17 in./43.2 cm deep.

Weight

15 lb/6.8 kg net, 23 lb/10.4 kg shipping.

Power

90 to 110V, 105 to 125V, 180 to 220V, or 210 to 250V; 50 to 400 Hz. Less than 45 watts.

NOTE

Specifications apply for settings from 1.00 to 9.99

SECTION 2
INSTALLATION AND INTERFACE

2.1 MECHANICAL INSTALLATION

After unpacking the instrument, visually inspect all external parts for possible damage to connectors, surface areas, etc. If damage is discovered, file a claim with the carrier who transported the unit. The shipping container and packing material should be saved in case reshipment is required.

The standard generator is a bench-top instrument with a collapsible tilt-bail to elevate its front end for convenient viewing.

The generator can also be rack mounted by attaching the rack mount adapters to the sides.

2.2 ELECTRICAL INSTALLATION

2.2.1 Power Connection

NOTE

Unless otherwise specified at the time of purchase, this instrument was shipped from the factory with the power transformer connected for operation on a 105 - 125 Vac line supply and with a ¾ amp slow-blow fuse.

Conversion for 90 to 110V, 180 to 220V, or 210 to 250V operation requires resetting two switches on the inside of the rear panel. To reset the switches, remove the top cover for access. Set the two switches and select the fuse for the ac line voltage according to the following table.

AC Line Voltage	Switch A	Switch B	Fuse (SB)
90 - 110	115	LO	3/4 amp
105 - 125	115	HI	3/4 amp
180 - 220	230	LO	3/8 amp
210 - 250	230	HI	3/8 amp

Connect the ac line cord to the mating connector at the rear of the unit.

2.2.2 Signal Connections

Use 50Ω shielded cables equipped with female BNC connectors to distribute 50Ω OUT, SYNC OUT, TRIG IN and VCG IN signals when connecting this instrument to associated equipment.

2.2.3 Control Connections

The remote (ASCII DATA IN/OUT) rear panel connection, harness wire colors, pin connections and signal names are given in Tables 2-1 and 2-2.

The remote connector is a Molex 03-09-1151 which mates with a Molex 03-09-2151 connector housing with up to 15 Molex 02-09-2118 pin contacts. Pin contacts are prepared using a Molex Model A6973 Crimping Tool to connect No. 18 or No. 22 wire (strip back 1/10 to 1/8 inch).

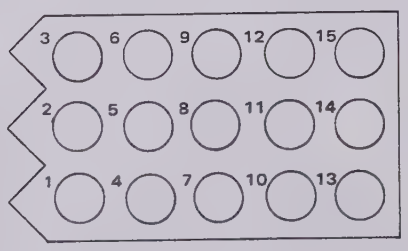

MOLEX 03-09-1151

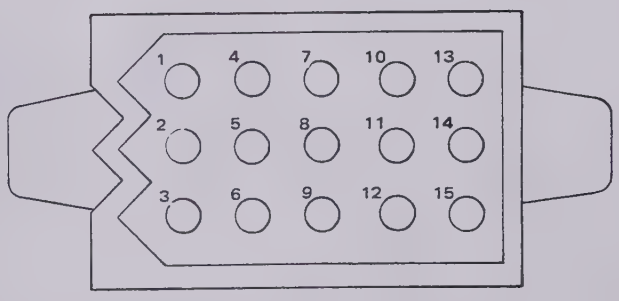

MOLEX 03-09-2151

Figure 2-1. Connectors (Socket/Pin Sides)

Table 2-1. ASCII DATA IN/OUT AND HARNESS CONNECTORS

	Connector					
	ASCII Data In/Out (Rear Panel)		Keyboard Harness		Display Harness	
Pin	Wire Color	Signal	Wire Color	Signal	Wire Color	Signal
1	1	PCOM				
2	2					
3	3	KINH	2	KINH		
4			1	+5V	7	+5V
5	5					
6	6	BUSY				
7	7	COM	91	COM	0	COM
8	8	XD2	8	KD2	1	DCLK
9	9	XD4	5	KD4		
10	90	XD3	3	KD3	2	DD0
11	91	XD1	7	KD1	4	DD2
12	92	XD5	4	KD5		
13	93	XD0	90	KD0	6	DSYNC
14	94	XD6	6	KD6	3	DD3
15	95	XCLK	9	KCLK	5	DD1

Code	Color	Code	Color
0	Black	8	Gray
1	Brown	9	White
2	Red	90	White with black tracer
3	Orange	91	White with brown tracer
4	Yellow	92	White with red tracer
5	Green	93	White with orange tracer
6	Blue	94	White with yellow tracer
7	Violet	95	White with green tracer

PCOM: Input Program Common
KINH: Keyboard Inhibit (When connected to pin 7)
COM: Signal Common
X: External
D: Data
0 - 6: Bits 0 thru 6
CLK: Clock
K: Keyboard
D: Display

Table 2-2. KEY, ASCII, HEXADECIMAL, AND BINARY CODES FOR PROGRAMMING FUNCTIONS

Control and Data Names	Model 159 Key	ASCII Character and TTY Keyboard	Hexa-Decimal Code	Binary (and ASCII Bus) XD6 Bit 7	XD5 Bit 6	XD4 Bit 5	XD3 Bit 4	XD2 Bit 3	XD1 Bit 2	XD0 Bit 1
Range (X 10 mult)*		(Space)	20	0	1	0	0	0	0	0
Invert phase/offset	CHS	–	2D	0	1	0	1	1	0	1
0	0	0	30	0	1	1	0	0	0	0
1	1	1	31	0	1	1	0	0	0	1
2	2	2	32	0	1	1	0	0	1	0
3	3	3	33	0	1	1	0	0	1	1
4	4	4	34	0	1	1	0	1	0	0
5	5	5	35	0	1	1	0	1	0	1
6	6	6	36	0	1	1	0	1	1	0
7	7	7	37	0	1	1	0	1	1	1
8	8	8	38	0	1	1	1	0	0	0
9	9	9	39	0	1	1	1	0	0	1
P-P amplitude	AMPL	A	41	1	0	0	0	0	0	1
Operating mode	MODE	B	42	1	0	0	0	0	1	0
Function (waveform)	FUNC	C	43	1	0	0	0	0	1	1
Reference offset	OFST	D	44	1	0	0	0	1	0	0
Range (X 10 mult)*	MULT	E	45	1	0	0	0	1	0	1
Frequency	FREQ	F	46	1	0	0	0	1	1	0
Unit select address	UNIT	G	47	1	0	0	0	1	1	1
Output on	ON	H	48	1	0	0	1	0	0	0
Output off	OFF	I	49	1	0	0	1	0	0	1

1 = True = Low
0 = False = High

*See the second entry of this control name.

SECTION 3
OPERATION

3.1 INITIAL CHECKOUT

To ensure that the generator is operating properly, make the power and interface connections (Section 2), and operate the generator, function-by-function, as described in the following paragraphs.

3.2 CONTROLS, INDICATORS AND PROGRAMMING

Programming instructions and considerations for the Model 158 and 159 generators are the same, except for keyboard enable control that only applies to the Model 159 generator.

The Model 159 has a 20-pushbutton front panel keyboard to provide the same control as the Model 159 or 158 20 remotely programmed ASCII character bytes.

The 20 generator controls and their various code conversions are listed in Table 2-2. The Model 159 front panel controls and indicators are shown in Figure 3-1.

3.2.1 Power

Power is turned on and off with the PWR pushbutton. When the power is turned on, the generator is automatically addressed and is ready to accept commands. If a different generator is to be addressed, use the UNIT control (refer to Paragraph 3.2.4). Also, when the power comes on, the output is automatically disabled to allow the loading of a program; line transients on the output are also avoided. The generator must get an ON command to provide an output (refer to Paragraph 3.2.5).

3.2.2 Indicators

The Model 159 indicators turn on to indicate the various functions, modes, quantities, sign, and address programmed; the numerals displayed are significant as frequency, amplitude or offset, but only one category at any one time. The 3-digit number is always a 1-digit whole number and a 2-digit decimal. The three digits are displayed in order of entry, shifting right-to-left as shown in Table 3-1. The single digit is a power of ten. (Only the last three entered significant

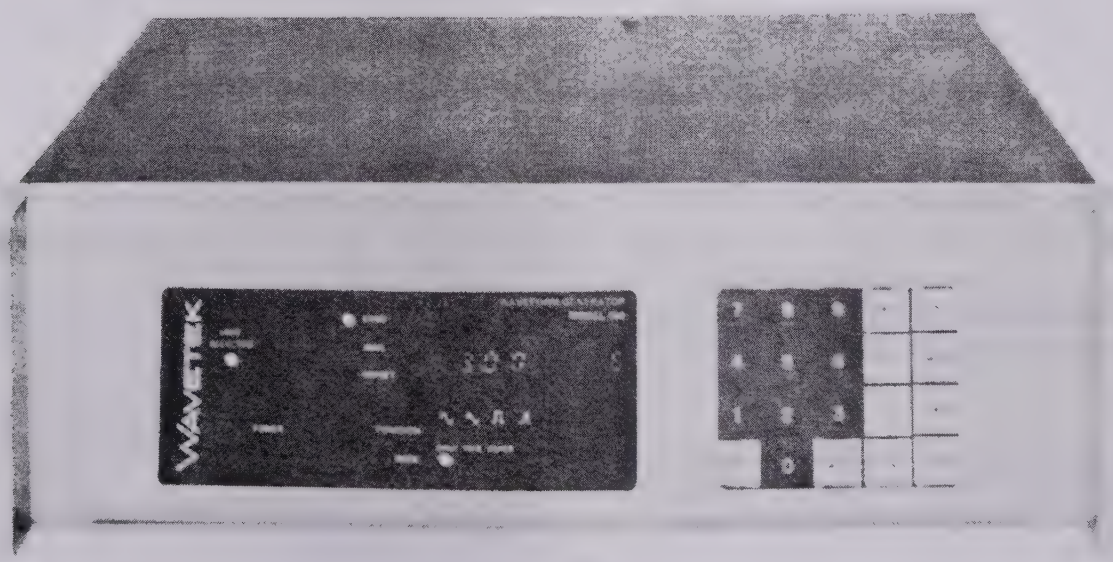

Figure 3-1. Model 159 Waveform Generator

digits and the last entered digit for the power of ten are stored. Any previously entered digits of the significant digits or the power of ten are shifted out of memory.)

3.2.3 Programming

Programming is mostly a matter of prefixing, by sequence, the numerical values and numeric codes with their intended use. For example, programming a continuous 5.79 kHz sine wave on Unit No. 1 is given in Table 3-1.

Table 3-1. EXAMPLE OF PROGRAMMING

Sequence	Wavetek Keyboard	Remote ASCII	Lighted Display
1	UNIT	G	---
2	1	1	SELECT
3	MODE	B	---
4	0	0	CONT
5	FUNC	C	---
6	0	0	∿
7	FREQ	F	---
8	5	5	0.05
9	7	7	0.57
10	9	9	5.79
11	MULT	E	---
12	3	3	3 (power of ten)

Table 3-2. KEYBOARD TO ASCII CONVERSION TABLE

Keyboard	ASCII	Keyboard	ASCII
AMPL	A	MULT	(Space) or E
UNIT	G	ON	H
OFST	D	OFF	I
MODE	B	0 thru 9	0 thru 9
FUNC	C	CHS	– (Minus)
FREQ	F		

Generally, alpha characters (A thru I) are subsection addresses and are usually followed by one or more numeric digits representing a value or control selection.

NOTE

Any character may be separated by spaces, periods or other characters not defined here. Spaces may be inserted between alpha control characters and numeric fields; however, a space will move from a value field to the exponent field where scientific notation is used after at least one numeric digit has been received. (See Paragraphs 3.2.8 and 3.2.9.)

The generators are designed to accept a scientific notation input format. System programmers using FORTRAN will find that the result of the format statement

20 FORMAT (1 HF, 1PE13.3)

will control the frequency without additional processing.

The following paragraphs describe the program elements and give their ASCII codes. The Model 159 front panel keys correspond one-for-one with the ASCII codes; if there is any doubt as to correspondence, refer to Table 3-2.

3.2.4 Unit Selected Address

After the unit prefix (G), program one digit to select the unit. The unit addressed in a multiple-unit group responds to subsequent commands; other units do not. Generators are given the address of 1 at the factory unless specified otherwise at the time of purchase. Address changes are easily made in the field. Subsequent instructions will be accepted by the last unit addressed.

3.2.5 Output On/Off

The generator output is enabled by programming H and inhibited by programming I. H and I connect and disconnect the generator output to the external BNC connector.

3.2.6 Operating Mode

Operating Mode	ASCII Character
Continuous	0
Triggered	1
Gated	2

After the mode prefix (B), program one digit to select the desired mode.

The generator output can be made to run continuously, triggered for just one cycle of waveform at a time, or gated for as many cycles or for as long as desired.

The triggered and gated modes require an external trigger level input at rear panel connector TRIG IN of at least +2V, not to exceed +50V; inputs below +2V are not to exceed –50V. In the triggered mode, one cycle of waveform is generated whenever the input at TRIG IN increases positively thru +2V.

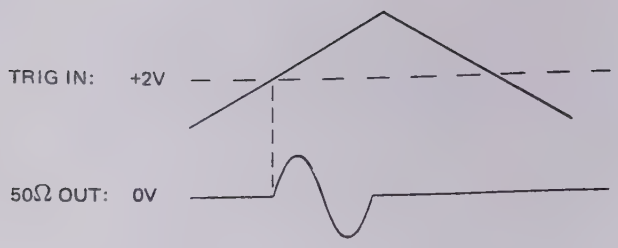

In triggered mode, the generator may be "manually" triggered by pressing the "1" key or programming an ASCII 1.

In the gated mode, waveforms are generated for as long as the input at TRIG IN stays above +2V. When the input at TRIG IN falls below +2V, the last cycle of waveform is completed and the waveform stops.

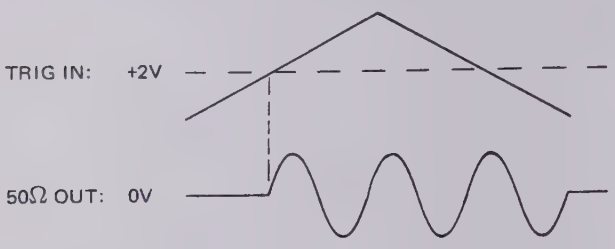

3.2.7 Function (Waveform)

Waveform	ASCII Character
Sine	0
Triangle	1
Square	2
Ramp	3

After the function prefix (C), program one digit to select the desired waveform. Waveforms can be inverted during amplitude selection.

3.2.8 Frequency and Multiplier

After the frequency prefix (F), program a 3-digit number (1.00 to 9.99) for the three most significant digits; after the multiplier prefix (E or space), program the power of 10 (0 thru 6).

3.2.9 Amplitude and Multiplier

After the amplitude prefix (A), program (–) if waveform inversion is desired; then, program a 3-digit number (0.00 to 9.99) for the three most significant digits. After the multiplier prefix (E or space), program the power of 10 (0, 1 or 2). Powers 1 and 2 are automatically accepted as –1 and –2. Amplitude is volts peak-to-peak into a 50Ω load.

NOTE

DC offset plus waveform peak value may not exceed 10V peak into an open circuit or 5V peak into 50Ω.

All waveforms including ramp have a center reference level. Notice the inversion caused by programming –V p-p. Normal waveforms start in the positive direction regardless of their offset. Inverted waveforms start in the negative direction regardless of their offset.

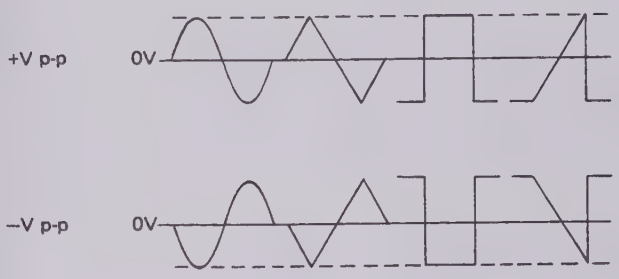

3.2.10 Signal Reference Offset

After the offset prefix (D), program (–) if negative offset is desired; then, program a 3-digit number (0.00 to 5.00) for the offset significant digits. The offset multiplier, or range, is the amplitude program multiplier. For example, if A150E1 and D350 are programmed, the waveform will be +0.15V p-p with an offset of +0.35V.

Offset control allows the generator output reference level to be offset, or displaced positive or negative to 5V. All waveforms including ramp have a center reference level from which the offset is made.

NOTE

DC offset plus waveform peak value may not exceed 10V peak into an open circuit or 5V peak into 50Ω.

3.3 OPERATING PROCEDURE

No preparation for operation is required beyond the completion of the initial installation checks. Allow the generator and associated equipment to warm up for specified generator accuracies. Refer to the control descriptions given in Paragraph 3.2 for actual keyboard or remote commands.

3.3.1 Operating as a Basic Waveform Generator

1. Terminate the 50Ω OUT connector with a 50Ω ±0.1% termination.

2. Select the desired waveform and continuous mode.

3. Select the desired frequency, output amplitude and offset.

NOTE

DC offset plus waveform peak value may not exceed 10V peak into an open circuit or 5V peak into 50Ω. Specifications apply for frequency and amplitude programs from 1.00 to 9.99.

3.3.2 Operating as a Voltage Controlled Generator

VCG operation is the same as the basic waveform operation plus the connection of a VCG voltage source to the VCG IN connector. Input impedance is 5 kΩ.

The VCG input can be used to externally control the frequency of the 50Ω OUT signal. A positive voltage applied to the VCG IN connector will increase the generator frequency, and a negative voltage will decrease the frequency. A 2.5V excursion can vary the frequency by a factor of 1000, and a 7.5V excursion will allow 300% overranging, as shown in the following table.

Range	1:3000 (300% Overrange)
10^0	0.01 Hz to 30 Hz
10^1	0.1 Hz to 300 Hz
10^2	1 Hz to 3 kHz
10^3	10 Hz to 30 kHz
10^4	100 Hz to 300 kHz
10^5	1 kHz to 3 MHz

The nomograph of Figure 3-2 shows the characteristics of the VCG circuit. Column A gives the 3-digit program setting; column B, the VCG IN voltage; and column C, the factor representing the resultant frequency of the generator (multiply by range for actual frequency). As an example of nomograph use, suppose you want to operate at a basic frequency of 350 kHz and vary the frequency by VCG voltage from 100 kHz to 2 MHz. Mark the 3.50 3-digit program setting in column A on the nomograph. Draw a line to each of the frequency limits in column C, 20.0 and 1.00. In the VCG IN Voltage column, the voltage range defined by these two lines is the VCG IN operating range. In the example, the VCG voltage range is from −0.60 to 4.15 volts.

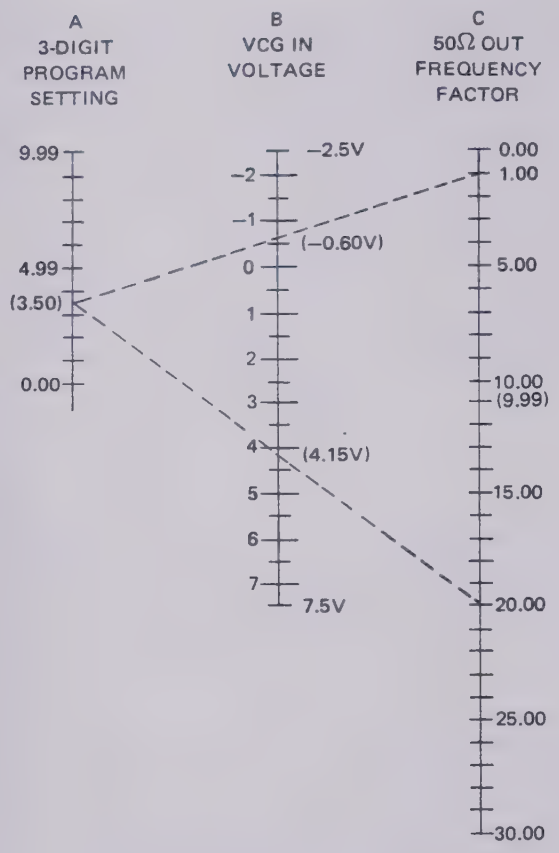

Figure 3-2. VCG Nomograph

3.3.3 Operating as a Triggered/Gated Waveform Generator

Trigger/gate operation is the same as the basic waveform operation plus the connection of a trigger source to the TRIG IN connector and the selection of TRIG or GATED mode, as applicable. The trigger/gate signal must be +2V, but less than ±50V. Input impedance is 1 kΩ. In triggered mode, the trigger signal will cause one cycle of output at the 50Ω OUT connector; in gate mode, the trigger signal will cause an integral burst of cycles lasting for the duration of the trigger signal plus the time required to complete the last cycle initiated during the trigger signal.

3.3.4 Operating as a DC Voltage Source

DC voltage output is not specified, but ±5V, 100 mA may be obtained by using offset voltage referred to the 0V level of the 50Ω OUT during the nontrigger time of trigger mode.

1. Terminate the 50Ω OUT connector with a 50Ω ±0.1% termination.
2. Select $\wedge\!\!\vee$ function and trigger mode.
3. Program 9.99 X 10^1 frequency.
4. Program 0.00 X 10^0 amplitude.
5. Ensure that no trigger signals are received.
6. Select the desired dc output by programming it as offset voltage.

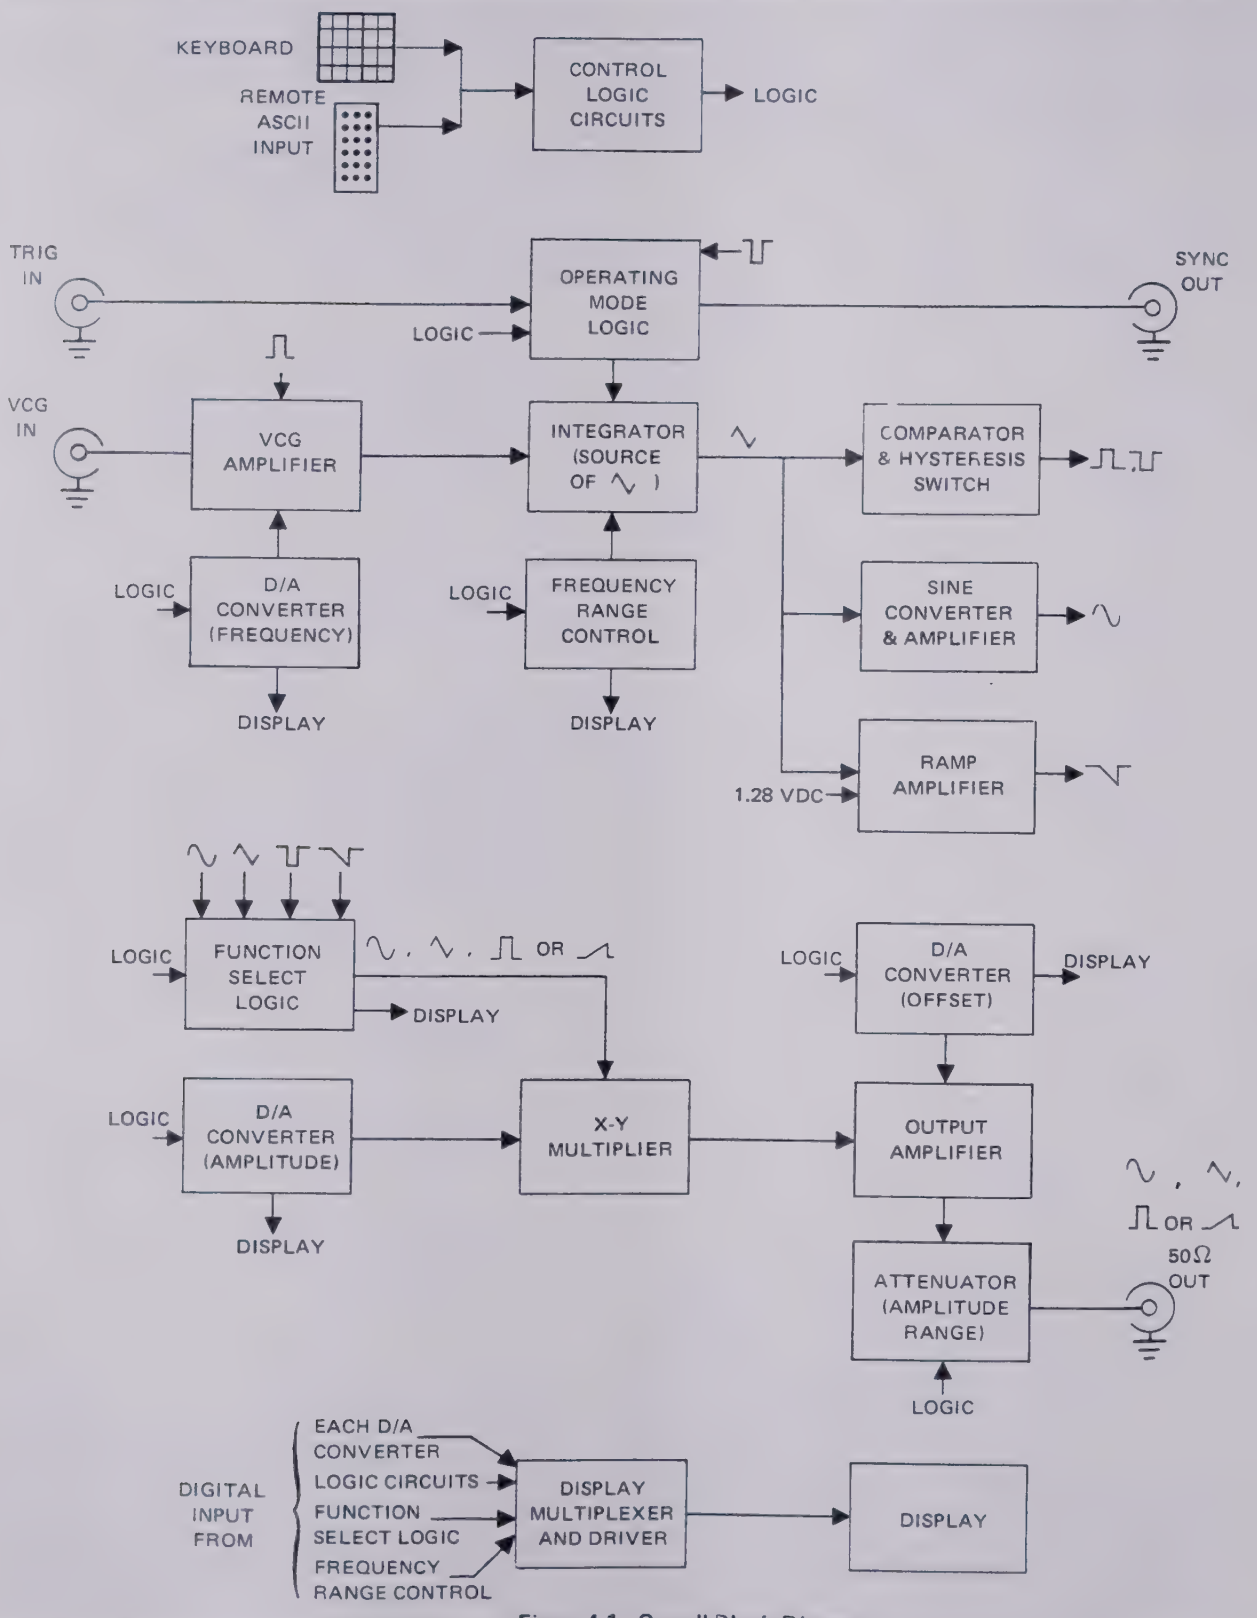

Figure 4-1. Overall Block Diagram

SECTION 4
CIRCUIT DESCRIPTION

4.1 LOGIC NOTATION AND TERMINOLOGY

To avoid confusion in determining logic states, please read and understand the following ground rules used in this manual.

1. On the schematics, all signals are true when high unless their mnemonics are overscored; the overscore indicates true-when-low.

2. Pulse and clock refer to transient change of state, whereas status refers to a logic state which requires new input to change.

4.2 BASIC OPERATION

The overall operation can be easily followed in Figure 4-1. All digital programmed inputs are via the keyboard or the remote ASCII connector. Two input BNC connectors are for the TRIG IN and VCG (voltage control of generator) IN signals. The outputs are selectable ∿ , ∿ , ⎍ or ⟋ waveform at the 50Ω OUT BNC. A sync output BNC is also provided for a TTL compatible square wave.

The integrator and comparator and hysteresis switch, acting upon each other, generate the basic waveforms of square and triangle. The mode of operation (triggered, gated or continuous) is logic controlled to act upon the integrator. Logic controls capacitance for generator frequency range and current, via a D/A converter and VCG amplifier, for specific frequency in the selected range. VCG IN voltage will also control frequency.

Diode arrays in the sine converter form the sine wave, and the square wave multiplexes the triangle wave and a voltage level to form the ramp waveform.

The waveform to be output is selected and multiplied with the selected amplitude, after which it is offset and attenuated as programmed.

The digital control data is multiplexed into the display bus for display panel illumination.

4.3 INPUT/OUTPUT

Seven-bit ASCII characters (see Table 2-2 and Drawing 158-200) and clock pulses are supplied to an ASCII data bus on the digital board thru the ASCII DATA IN/OUT connector or supplied by the keyboard to the digital board. (Generators with options will accept and convert other data formats. Once converted, the data is placed on the ASCII data bus.) The character bits are 0 to 0.4 volt for a binary 1 and $\geqslant$ 2.4V, $<$ 5.0V or open for a binary 0. The character bits are designated D0 thru D6 and prefixed as to their type; i.e., X for in/out external, K for keyboard, and OPT for optional interface conversion.

The ASCII data bus is that set of eight lines handling D0 thru D6 and CLK. Keyboard input J2 is always a part of the bus as well as the termination socket XIC41 (shown in Drawing 158-218, Sheet 1).

Non-ASCII signals to the generator are VCG IN, which is connected to the analog board via the digital board, and TRIG IN, which goes to the trigger logic on the digital board. The generator main output signal is from the analog board to the rear panel 50Ω OUT BNC connector; this signal is a selectable ∿ , ∿ , ⎍ or ⟋ that can be offset, inverted and varied in amplitude. The SYNC OUT signal is a fixed amplitude square wave that is TTL compatible.

4.4 INTERFACE (Drawing 158-218, Sheet 1)

By means of jumpers (Drawing 158-218, Sheet 1), the standard model signals bypass the option card connector J4, allowing J9 (ASCII DATA IN/OUT) to be connected directly to the ASCII data bus. The ASCII data bus may extend thru several instruments. In any case, the integrated circuit termination pack should be inserted only once on the ASCII data bus and at the far end of the bus from the keyboard or control device.

4.5 KEYBOARD (Drawing 159-216)

The keyboard transmits pressed-key data plus a clock pulse to the ASCII data bus. Proper time alignment of the seven data bits and clock is maintained by the IC9 clock circuit driving IC5, a binary counter, to generate a time code. The

counter and the decoder chips (IC3 and IC7C) select a column of keys that are scanned by the multiplexer IC4 to generate time "windows" for the data bits corresponding to each key function. IC4 outputs transmit the status of the selected input. For example, between IC5 count 0 and 1, a 7-bit code for key 0 is generated and ready to be placed on the ASCII data bus if the 0 key is pressed. If the key is pressed, the binary counter IC5 stops and the seven bits plus a clock pulse are placed on the data bus. When the key is released, the windows for keys 1, 2, 3, etc., are generated in sequence.

4.6 DIGITAL BOARD CONTROL LOGIC (Drawing 158-218, Sheet 2)

The stream of ASCII characters (seven parallel bits per character) is decoded into hexadecimal data. This data is then distributed throughout logic control circuitry to program all of the holding registers which control the operation of the generator. Refer to Table 2-2 for conversion of programmed signals, keyboard, hexadecimal, binary and logic bit terminology.

Four types of clock pulses are generated to categorize the bits of data: alpha clock, numerals clock, minus sign clock and range clock. These clock signals, along with the data bits, cause explicit control signals to be generated.

Control logic consists of the following collection of logic blocks:

1. Binary to hexadecimal conversion (0 thru 9, D, 20, 30 and 40)
2. Unit Enable (ITSME)
3. Minus Sign Clock (MCLK)
4. Alpha (Except Multiplier) Clock (40EC)
5. Numerals Clock (30C)
6. Numeral Enables
7. Range (X 10 Multiplier) Clock (RNGCLK)
8. Display Digits Reset (ADRSET)
9. Minus Sign Enable (MSIGN)
10. On/Off Control (ENABLE)
11. Two-Star Converter (D0* thru D3*)
12. Turn-On Reset (RESA, RESB)
13. Trigger Clock (TRIGC)
14. Mode Select (M0, M1)
15. Manual Trigger
16. Generator Enable ($\overline{\text{OPERATE}}$)
17. Function Select (F0, F1)

4.6.1 Binary to Hexadecimal Conversion (0 thru 9, D, 20, 30 and 40)

The seven bits of character and one clock bit are converted to hexadecimal code. The four least significant bits are converted to a decimal number from 0 thru 9 or D. The three most significant bits are converted to 20, 30 or 40 and enabled for the duration of the clock pulse. See the hexadecimal column in Table 2-2. As shown in the table, 2D is ASCII minus and 20 is ASCII space. Then, on the schematic 20 with D is minus and 20 with 0 is space (the space is one of two multiplier addresses). Hexadecimal 30 with 0 thru 9 are the result of numeric data, and hexadecimal 40 with 0 thru 9 are the result of alpha data.

4.6.2 Unit Enable (ITSME)

A jumper from E24 or E25, etc., to E29 determines the address of the generator as 1, 2, etc. When unit select and a number are programmed, and the number is the correct unit address, ITSME status is generated. ITSME enables alpha and numerals clock and the display.

4.6.3 Minus Sign Clock (MCLK)

MCLK is generated when a phase inversion or negative offset is programmed (ASCII –).

4.6.4 Alpha (Except Multiplier) Clock (40EC)

If the correct generator is addressed and any alpha other than multiplier is input, a clock pulse is generated (40EC and $\overline{\text{40EC}}$). This signal is used to clock all alpha related functions except the range (or X 10 multiplier). ITSME enables.

4.6.5 Numerals Clock (30C)

Numerals clock (30C) is used to distinguish between alphas

nd numerics and to clock numeric related functions.

4.6.6 Numeral Enables

This circuit triggers the display digit reset one-shot and enables a portion of the range clock circuit only for the numeral programmed immediately after an alpha (except range). Output is

Numeral = High
Alpha = Low

4.6.7 Range (X 10 Multiplier) Clock (RNGCLK)

If a numeral was last programmed, an ASCII space programmed will generate a range clock pulse (RNGCLK). Or, if range (ASCII E) is programmed, a range clock pulse is generated. This pulse is used to set the range gate to enable the frequency range logic and the amplitude attenuator logic.

4.6.8 Display Digits Reset (ADRSET)

A high following a low from the numerals enable circuit triggers a 100 ns ADRSET pulse. This pulse is used to clear the registers for the display digits. Therefore, a numeral programmed after an alpha, such as frequency or amplitude, causes the registers to be cleared, but another programmed numeral will not cause the registers to clear.

4.6.9 Minus Sign Enable (MSIGN)

MSIGN status is generated on the falling edge of MCLK; that is, an inverted phase or offset has been programmed. MSIGN status is removed when an alpha is generated. MSIGN is used to change the polarity of the amplitude or offset.

4.6.10 On/Off Control (ENABLE)

The 50Ω OUT output is enabled when output-on is programmed. Output-on (ASCII H) generates ENABLE and $\overline{\text{ENABLE}}$. Output-off (ASCII I) inhibits ENABLE and $\overline{\text{ENABLE}}$.

4.6.11 Two-Star Converter

	Decimal									
	0	1	2	3	4	5	6	7	8	9
XD0		H		H		H		H		H
XD1			H	H			H	H		
XD2					H	H	H	H		
XD3									H	H
XD0*		H		H		H		H		H
XD1*			H	H			H	H	H	H
XD2*					H	H	H	H	H	H
XD3*									H	H

4.6.12 Turn-On Reset (RESA, RESB)

This one-shot multivibrator clears or presets all necessary holding registers at power-on time.

4.6.13 Trigger Clock (TRIGC)

When the operating mode is programmed (ASCII B), the gate IC49 is enabled in order for the following programmed numerals clock pulse (30C) to generate the trigger clock pulse ($\overline{\text{TRIGC}}$). This pulse is used to gate the manual trigger D0 binary data bit and clock bits $\overline{1}$ and $\overline{2}$ of mode numerics at the mode select circuit to generate M0 and M1.

4.6.14 Mode Select (M0, M1)

$\overline{1}$	$\overline{2}$	MODE	M0	M1
H	H	CONT	L	L
L	H	TRIG	H	L
H	L	GATE	L	H

Numerics $\overline{1}$ and $\overline{2}$ determine status of M0 and M1 when clocked by $\overline{\text{TRIGC}}$. These status signals define the operating mode of the generator in the trigger circuit and display.

4.6.15 Manual Trigger

After the trigger mode is programmed, any subsequent programmed ASCII binary bit D0, such as the numeral 1, will generate another $\overline{\text{TRIGC}}$; the combination of $\overline{\text{TRIGC}}$ and D0 is a manual trigger pulse. The manual trigger rate must be slower than the generator frequency.

4.6.16 Generator Enable ($\overline{\text{OPERATE}}$)

See Paragraph 4.6.14 for M0 and M1 status for a given mode.

Continuous Mode. If continuous mode is programmed, M0 and M1 are low which holds $\overline{\text{OPERATE}}$ low, allowing the generator to run.

Gated Mode. In gated mode, M0 is low and M1 is high. Trig-mode gate is held high; gate-mode gate is gated and will respond to a trigger signal. When TRIG is high, $\overline{\text{OPERATE}}$ is low. When TRIG is low, the low is removed from the IC40B clear, and the completion of the SQR square wave at the IC40B clock input causes $\overline{\text{OPERATE}}$ to be high.

Triggered Mode. In triggered mode, M0 is high and M1 is low. Gated-mode gate is held high; trig-mode gate is gated and will respond to the TRIG or manual trigger signal. A trigger causes the trig-mode gate to go high, allowing $\overline{\text{OPERATE}}$ to be low. $\overline{\text{OPERATE}}$ feedback to IC40A removes the clear on IC40B and upon the completion of the SQR square wave at the IC40B clock input causes $\overline{\text{OPERATE}}$ to go high.

4.6.17 Function Select (F0, F1)

When the alpha for function is programmed (ASCII C), the gate IC49 is enabled in order for the following programmed numerals clock pulse (30C) to clock ASCII binary bits D0 and D1. D0 and D1 are the least significant bits of the programmed numeral. (0 = ∿ , 1 = ⩘ , 2 = ⎍ and 3 = ⩙ .) Outputs are as noted on the schematic.

4.7 FREQUENCY D/A LOGIC (Drawing 518-218, Sheet 6)

The programming of the frequency alpha (ASCII F) enables the clearing and clocking gates for the frequency numeric data holding registers. The programming of a numeral following the frequency alpha will clear the registers and enter the data in the LSD register. Subsequent programmed numerals will be entered serially without any clearing action. Output data of the registers controls the diode gates, which switch current thru weighting resistors into a summing node of an amplifier to create the analog voltage labeled D/F. The register output data is also used for display information.

If the range alpha (ASCII E) is programmed and frequency was the last programmed alpha, the frequency clearing and clocking gates are disabled and the gate for the range data holding register is enabled. Subsequent programmed numerals will enter the data at the range data holding register input. The outputs FR0, FR1 and FR2 of this register are decoded to decimal data which are used to control relays for selected range capacitors and frequency adjustment controls (see Schematic 158-219 and Paragraph 4.12.5). FR0, FR1 and FR2 are also used as display information.

4.8 OFFSET D/A LOGIC (Drawing 158-218, Sheet 5)

The programming of the offset alpha (ASCII D) enables the clearing and clocking gates for the offset numeric data holding registers. The programming of a numeral following the offset alpha will clear the registers and enter data in the LSD register. Subsequent programmed numerals will be entered serially without any clearing action. Output data of the registers controls the diode gates, which switch current thru weighting resistors into a summing node of an amplifier to create the analog voltage labeled DC OFFSET. The register output data is also used for display information.

If inversion is programmed (ASCII –) following offset, MOFFSET is generated which causes the electronic SPDT switch to control the polarity of the selected offset voltage.

4.9 AMPLITUDE D/A LOGIC (Drawing 518-218, Sheet 4)

The programming of the amplitude alpha (ASCII A) enables the clearing and clocking gates for the amplitude numeric data holding registers. The programming of a numeral following the amplitude alpha will clear the registers and enter the data in the LSD register. Subsequent programmed numerals will be entered serially without any clearing action. The output data of the registers controls the diode gates, which switch current thru weighting resistors into a summing node of an amplifier to create the analog voltage labeled D/V. The register output data is also used at the display driver circuit.

If the range alpha (ASCII E) is programmed and amplitude was the last programmed alpha, the frequency clearing and clocking gates are disabled and the gate for the range data holding registers clock is enabled. Subsequent programmed numerals will enter numeric data at the range data holding register inputs with the following results:

$\overline{1}$	$\overline{2}$	–20 dB	–40 dB	0 dB
H	L	L	H	L
H	H	L	L	H
L	H	H	L	L

Where 0 dB = X 10^0 multiplier
–20 dB = X 10^{-1} multiplier
–40 dB = X 10^{-2} multiplier

Normal waveform phase has been set by the function select circuit signal F1 in the following manner:

Function	F1	MAMPL	Q7	Q8	Normal-Phase D/V Polarity
∿	L	L	On	Off	+
⩘	L	L	On	Off	+
⎍	H	H	Off	On	–
⩙	H	H	Off	On	–

If inversion is programmed (ASCII –) following the amplitude alpha, MAMPL status is reversed, causing the electronic DPST switch controlling Q7 and Q8 to reverse the polarity of the analog signal D/V. D/V controls 50Ω OUT signal amplitude and polarity at the X-Y multiplier (see Schematic 518-219 and Paragraph 4.12.7).

4.10 DIGITAL BOARD DISPLAY (DRIVER) LOGIC (Schematic 158-218, Sheet 3)

All of the status data from the holding registers are accumulated and multiplexed into the display logic. By multiplexing, the data is transferred to the display in a minimum amount of lines (DD0 thru DD3) and then is decoded on the display board. To synchronize the transferred data, a sync ($\overline{DSYNC}$) line and clock ($\overline{DCLK}$) pulse are provided for both multiplexing and decoding.

4.10.1 Clock and Multiplex Time Code

The divide-by-9 binary counter IC37, clocked at a 5 kHz rate, supplies the necessary time codes (K0, K1, K2, K3) for multiplexing the display data. The same 5 kHz clock also drives the clock pulse DCLK for the display.

4.10.2 Select Frequency, Amplitude or Offset Display

$\overline{SELF}$	$\overline{SELA}$	$\overline{SELOFF}$	SD0	$\overline{SD0}$	SD1	$\overline{SD1}$
L	H	H	H	L	L	H
H	L	H	L	H	L	H
H	H	L	L	H	H	L

The SELF, SELA and SELOFF status signals from their respective D/A circuits generate the SD0 and SD1 codes which enable frequency, amplitude, offset, range or minus sign data for multiplexing. Because amplitude, frequency and offset share the same numerical display, this code necessarily ensures that only one set of data is enabled at a time.

4.10.3 Amplitude, Frequency and Offset Multiplexing

All three of the multiplexer outputs are paralleled and connected to the display bus thru the 2-star decoder. The three multiplexer chips, frequency, amplitude and offset, receive input data from the holding registers of their respective D/A converters. The multiplexers are enabled by the programming of frequency, amplitude or offset, which generate SD0 and SD1, and by time code $\overline{K2}$. In a specific multiplexer, the three groups (A, B and C) of four data bits each are placed on the bus (DD0, DD1, DD2 and DD3) by time codes K0 and K1. See the chart on the schematic and the ABC versus K0, K1 matrix on the multiplexer itself for logic and states and timing. The 2-star decoder converts the 2-star bit weighting back to conventional binary (see 2-star converter, Paragraph 4.6.11).

4.10.4 Amplitude and Frequency Range (X 10 Multiplier) Multiplexing

In the multiplexer A groups, −20 and −40 dB are amplitude attenuation, while FR bits of the B group are frequency selection bits. The A group or the B group is enabled for multiplexing by SD0, which is high for frequency display and low for amplitude and offset. Multiplexing is controlled by time codes $\overline{K0}$, $\overline{K1}$ and $\overline{K2}$ (see the chart on the schematic).

4.10.5 Minus Signs, Function and Enable, and Mode and Unit Select Multiplexing

Multiplexing of the following signals is controlled by K2, $\overline{K0}$ and $\overline{K1}$, as shown on the schematic chart.

The minus sign for amplitude is gated by the selection of amplitude for display, $\overline{SD1}$ and $\overline{SD0}$ high. The minus sign for offset is gated by the selection of offset for display, $\overline{SD0}$ and SD1 high. 0 dB or SD0 high (the selection of frequency) will be used to inhibit the range minus sign for frequency and 0 dB amplitude. SD0 and SD1 states are used to light the display mode LEDs. F0 and F1 states are used to light the function (waveform) LEDs. $\overline{ENABLE}$ is used to enable the display of the function symbol. M0 and M1 states cause the operating mode LEDs to light. ITSME causes the UNIT SELECTED LED to light.

4.10.6 Display Enable

Some systems may have several instruments connected to one display. Display enable ensures that only one instrument at a time drives the display. If this unit is selected ($\overline{ITSME}$), its display data will be gated. If it is not selected, but power is on, the subsequent K3 edge will cause a low to be generated, disabling the display data output.

4.11 DISPLAY LOGIC (Drawing D158-217)

The display board receives the multiplexed data character (bits DD0 thru DD3) from the digital board. At each character time, the bits represent one of the following display items or groups:

Data	Display	Enable Signal	Data Bits
Range Digit	DS1	DIG9	DD0 - DD3
Most Significant Digit	DS2	DIG1	DD0 - DD3
Middle Digit	DS3	DIG2	DD0 - DD3
Least Significant Digit	DS4	DIG3	DD0 - DD3
Display Mode	CR11 - CR13	DIG4	DD2 - DD3
3-Digit-Value Minus Sign	DS8	DIG4	DD0
X 10 Multiplier Minus Sign	DS7	DIG4	DD1
Function (Waveform)	CR1 - CR4	DIG5	DD0 - DD3
Operating Mode	CR8 - CR10	DIG6	DD0 - DD2
Unit Select	CR17	DIG6	DD3

The routing of the correct data to the correct display is determined by the clock pulse shifting the XSYNC bit thru the 9-bit parallel output shift register. The shift register outputs (DIG1 thru DIG9) enable the clock signal to clock the multiplexed data bits into the proper display holding registers at the proper time, thus correctly routing and de-skewing the data bits.

4.12 ANALOG BOARD (Drawing 158-219)

4.12.1 Generator Loop

The purpose of this loop is to generate symmetrical triangle and square waves simultaneously.

Control of current direction for capacitor C (Figure 4-2) charging is determined by whether diode switch CR1 (IC14-7) is forward biased (turned on) or reverse biased (turned off). Resistors R22, R40, R45, R52, R58 and R73 are matched to ensure equal currents.

When the voltage at point A is positive, diode CR1 is forward biased and CR2 is reverse biased. When CR1 is forward biased by the positive cycle of the square wave, current 2I (twice I) pulled by the 1st VCG amplifier comes from the square wave source. Because CR2 (IC14-6) is reverse biased, the current I from the 2nd VCG amplifier is charging the capacitor C which causes the voltage at point B to decrease linearly. As soon as the voltage at point B reaches −1.25V, the output of the hysteresis switch will switch to a negative voltage. CR1 becomes reverse biased and CR2 becomes forward biased. The current pulled by the 1st VCG amplifier (2I) is now comprised of the current from the 2nd VCG amplifier (1I) and exactly 1I from the capacitor C, which is the same amount as its charging current. The voltage at point B will increase. Again the hysteresis will switch positive when the voltage at point B reaches +1.25V. Thus, the triangle and square wave signals are generated simultaneously.

4.12.2 VCG Amplifier

The output frequency depends on the size of the capacitor selected and the amount of current I charging the capacitor. The magnitude of the current is controlled by the VCG amplifiers, which in turn are controlled by the voltage from the frequency D/A amplifier and the VCG input.

4.12.3 Sine Converter and Amplifier

The triangle is shaped into a sine wave thru three diode networks utilizing the nonlinearity of the diodes. The outputs of these diode networks are summed and amplified in the sine amplifier.

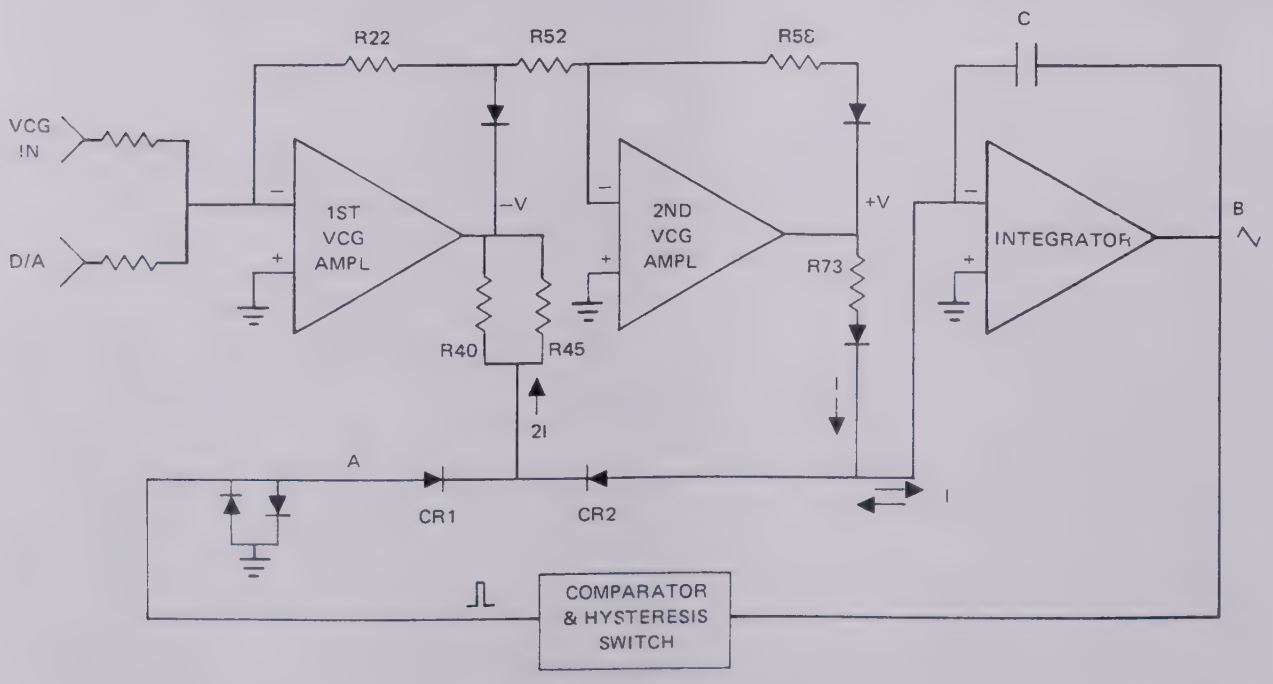

Figure 4-2. Generator Loop

4.12.4 Ramp Amplifier

A square wave from the comparator circuit (Figure 4-3) alternately enables the negative triangle ramp thru IC8A and the +1.25V from R64 thru IC8B to form the ramp waveform. The output resultant is +1.25V during one half cycle and the negative going portion of the triangle during the other half portion.

4.12.5 Frequency Range Logic

FR0	FR1	FR2	Power of 10
L	L	L	0
H	L	L	1
L	H	L	2
H	H	L	3
L	L	H	4
H	L	H	5
L	H	H	6
H	H	H	7

This circuit contains a binary to decimal decoder, which converts three lines of input data (FR0, FR1, FR2) to a one-line-of-eight output in order to drive the frequency range multiplier relays and control adjustments. FR0, FR1 and FR2 originate from holding register IC23 on the digital board (see Frequency D/A Logic, Paragraph 4.7).

4.12.6 Function Selector

$\overline{F0}$	$\overline{F1}$	Function
H	H	∿
L	H	∿
H	L	⎍
L	L	⎍

Selection of each waveform is accomplished by electronic switches. See Digital Board Schematic 158-218, Sheet 2, and Paragraph 4.6.17 for the origin of $\overline{F0}$ and $\overline{F1}$.

4.12.7 X-Y Multiplier and Output Amplifier

The selected waveform is fed into one input of the X-Y multiplier and a control voltage from the amplitude D/A amplifier is fed to the other input. Refer to Figure 4-4. The differential output from the X-Y multiplier is directly proportional to the product of the two inputs. One of the differential outputs is fed thru an inverting amplifier and then summed into a second inverting amplifier along with the other differential output from the x-y multiplier. The combined operation of these two inverting amplifiers is equal to one differential amplifier. Waveform inversion and addition is as shown in Figure 4-4.

4.12.8 Attenuator Select Logic

Attenuation of 0 dB, −20 dB or −40 dB is accomplished by selecting one-of-three range relays and an enable relay allowing the output amplifier to be enabled or disabled to the 50Ω OUT connector.

4.12.9 Generator Enable

The triangle generator loop will free run continuously only if the $\overline{\text{OPERATE}}$ voltage is low. Refer to Figure 4-5. When the $\overline{\text{OPERATE}}$ voltage is high, the output of the integrator will be clamped to the input, which stops the generator from free running. The J-K flip-flop is used to control the timing so that the triangle will always stop at the end of the cycle. The triangle will stop at time t_3 if $\overline{\text{GATE ENABLE}}$ is reset high between times t_1 and t_2 as shown in the timing diagram of Figure 4-5. $\overline{\text{OPERATE}}$ originates from the digital board generator enable circuit (refer to Schematic 158-218, Sheet 2, and Paragraph 4.6.16).

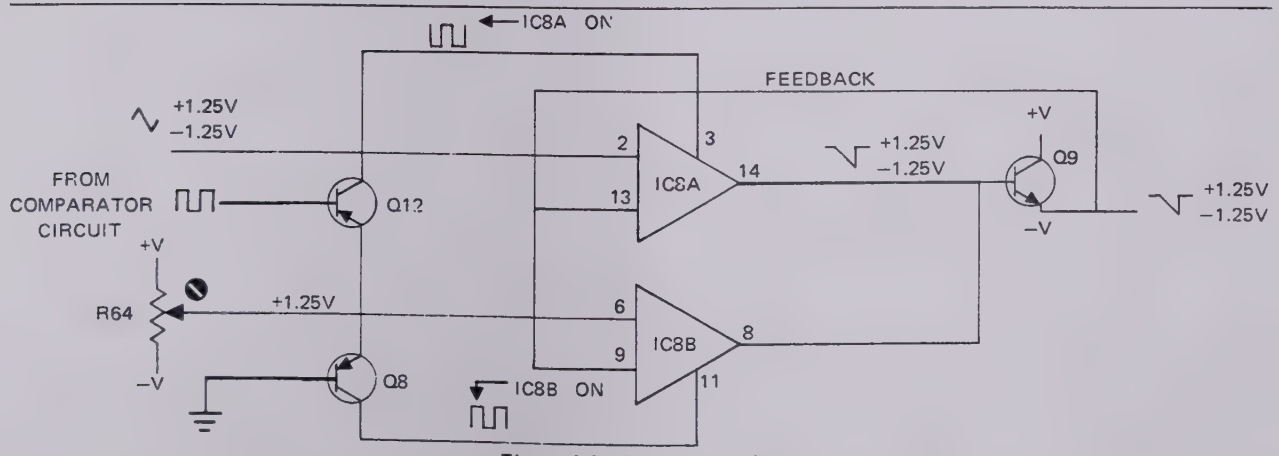

Figure 4-3. Ramp Amplifier

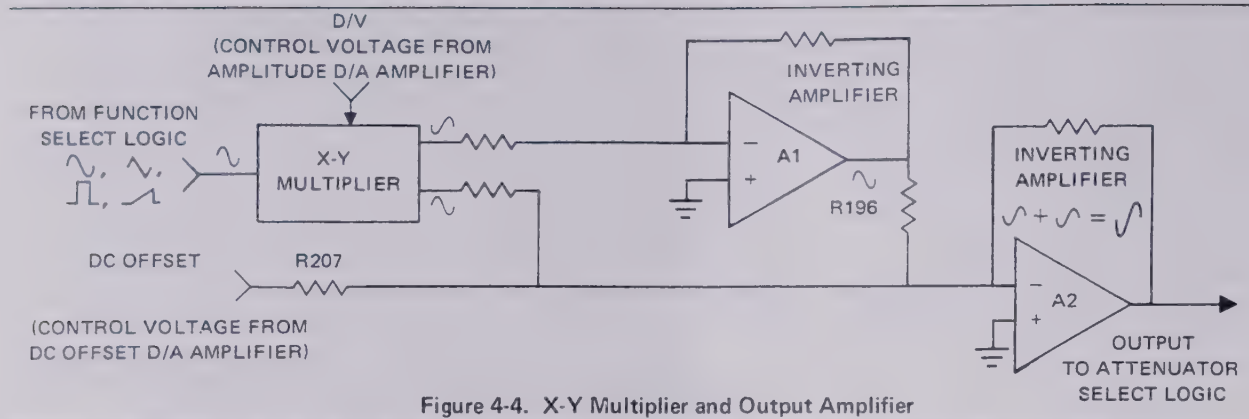

Figure 4-4. X-Y Multiplier and Output Amplifier

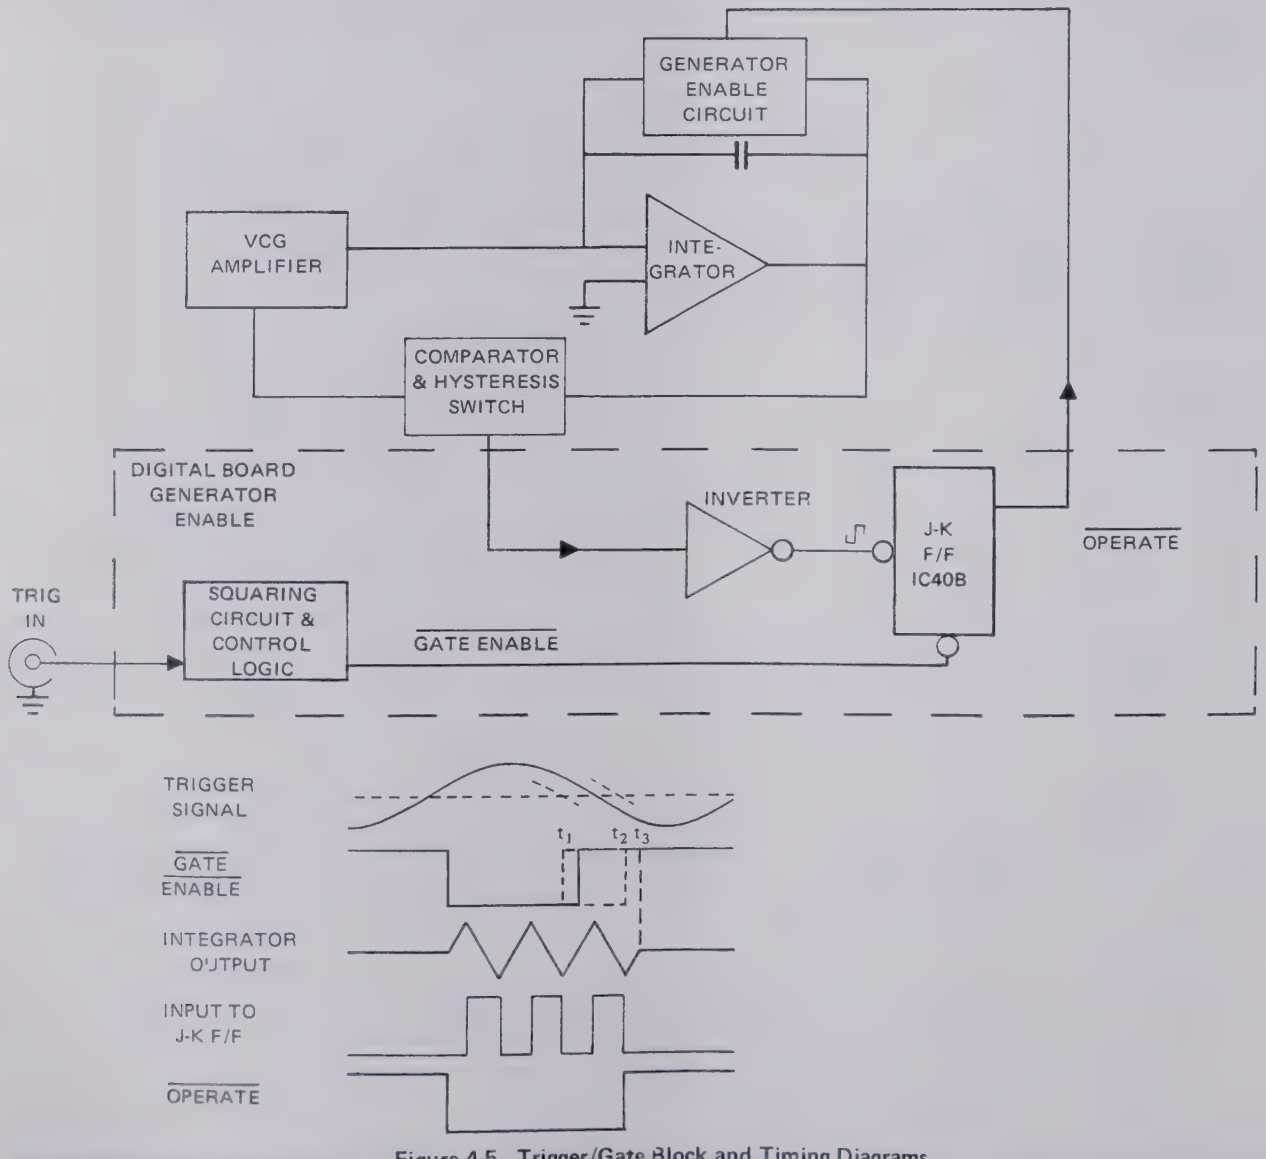

Figure 4-5. Trigger/Gate Block and Timing Diagrams

SECTION 5
CALIBRATION

After referring to the following preliminary data, perform calibration, as necessary, per Table 5-1. If performing partial calibration, check previous settings and adjustments for applicability.

1. Refer to calibration drawing, Figure 5-2, and calibration chart (Table 5-1).

2. Unless otherwise noted, all measurements made at the 50Ω OUT connector should be terminated into a 50Ω (±0.1%) load.

3. TPs (Test Points) and adjustments are prefixed as follows:

   A1 – Power Supply
   A2 – Digital Board
   A3 – Analog Board

4. Before connecting the unit to an ac source, check the ac line circuit to make sure the 115/230 and HI/LO switches are set at the correct position (see Paragraph 2.2.1).

5. Start the calibration by setting the front panel switches or program for the following:

Power	On
Unit Select	Select unit to be calibrated
Mode	Continuous
Frequency	9.99E2
Amplitude	9.99E0
Offset	0.00
Function	∿
Output On/Off	On

6. Allow the unit to warm up at least 30 minutes for final calibration.

Table 5-1. CALIBRATION CHART

Check	Tester	Calibrated Points	Program	Seq	Control	Desired Results	Remarks
Power Supply Regulation	Voltmeter	A3TP2 (+15V), A3TP1 (Gnd)	See initial conditions.	1	A1R24	+15V ±20 mV	
		A3TP3 (–15V), A3TP1		2	–	–15V ±50 mV	
		A3TP4 (+5V), A3TP1		3	–	+5V ±250 mV	
Triangle Amplitude	Oscilloscope	A3TP5, A3TP1 (Gnd)		4	A3R59	+1.25V ±5 mV	
		A3TP5, A3TP1		5	A3R62	–1.25V ±5 mV	
Symmetry	Oscilloscope	50Ω OUT	Func ⎍ Freq 0.10E4	6	A3R16	Minimum frequency change*	*While opening and shorting VCG IN to BNC case.
				7	A3R90, A3R17*	Time symmetry error <1%	*Use if necessary for adjustment of proper frequency.
			Freq 0.01E4	8	A3R44, A3R17*	Time symmetry error <1% Frequency <100 Hz	*Use if necessary for adjustment of proper frequency. Repeat 7 and 8, as necessary, for optimum results.

Table 5-1. CALIBRATION CHART (Continued)

Check	Tester	Calibrated Points	Program	Seq	Control	Desired Results	Remarks
Frequency	Counter	SYNC OUT	Freq 9.99E3	9	A3R2	9.99 kHz	
			9.99E5	10	A3C33	999 kHz	
			1.00E3	11	A3R17	1.00 kHz	Repeat 9, 10 and 11 for optimum results.
			0.00E3	12	A3R17	<10 Hz	If adjustment is made, repeat 11.
			9.99E0	13	A3R15	9.99 Hz	
			9.99E1	14	A3R11	99.9 Hz	
			9.99E2	15	A3R6	999 Hz	
			9.99E4	16	A3C15	99.9 kHz	
			3.00E6	17	A3R5	3.00 MHz	
			1.00E6	18	A3R5	1.00 MHz	Repeat 17 and 18 for optimum results.
X-Y Multiplier	Oscilloscope	A3TP5, A3TP1 (Gnd)	Func ∿ Freq 9.99E2 Ampl 0.00E0 Ofst 0.00 Mode Trig	19	A3R119	0V ±5 mV	
		50Ω OUT	Short A3TP5 to A3TP1	20	A2R28	Minimum voltage shift (±5 mV)	Obtain minimum voltage shift when switching between + and − offset. Adjust A3R217 to keep voltage at zero.
			Ampl 0.00	21	A3R182	<10 mV	
			Ampl 9.99	22	A3R182	<10 mV	Recheck 21. Readjust A3R217 to keep voltage at zero.
			Remove A3TP5 short Ampl 0.00E0 Mode Cont	23	A3R186	Minimum signal	
			Ampl 0.02E0	24	A3R201	Most linear triangle waveform	
			Ampl 0.00E0	25	A3R186, A2R99	Minimum + and − amplitude	Obtain minimum signal in both + and − amplitude.

Table 5-1. CALIBRATION CHART (Continued)

Check	Tester	Calibrated Points	Program	Seq	Control	Desired Results	Remarks
Sine Distortion	Oscilloscope, LF Sine Distortion Amplifier with X 1 probe	A3TP5*	Func ∿ Ampl 9.00E0	26	A3R137, A3R138	Minimum sine distortion	*See Figure 5-1 for test setup.
		50Ω OUT		27	A3R190	Minimum sine distortion	Typically <0.2%. See Figure 5-1 for test setup.
			Freq* 9.99E3 9.99E2	28	A3R137, A3R138, A3R190	Minimum sine distortion	*Optimize for both settings.
				29			Repeat 19 thru 23.
Output Amplitude and DC Offset	Voltmeter	50Ω OUT	Short A3TP5 to A3TP1 Func ∿ Ampl 0.00E0 Ofst 5.00 Mode Trig	30	A2R30	+5.00 Vdc ±10 mV	
			Ofst –5.00	31	A2R34	–5.00 Vdc ±10 mV	
			Ofst 0.00	32	A2R28	Minimum voltage shift (<5 mV)*	*While switching from + and – dc offset. Adjust A3R217 to keep voltage at zero.
				33			Repeat 30, 31 and 32 to optimize.
			Remove A3TP5 short Ampl 9.99E0 Mode Cont	34	A2R107	9.99V p-p ∿ ±10 mV	
			Ampl–9.99E0	35	A2R111	9.99V p-p ∿ ±10 mV	
			Func ⎍ Ampl 9.99E0	36	A3R55, A3R48	±5.00V peak ±10 mV	
			Ampl–9.99E0	37	A3R55, A3R48	50% of observed error*	*Split error with 36.
			Func ∿	38	A3R98, A3R116	±5.00V peak ±10 mV	R98 - Amplitude R116 - Symmetry
			Func ◿	39	A3R79, A3R64	±5.00V peak ±10 mV	R79 - Symmetry R64 - Separation

Table 5-1. CALIBRATION CHART (Continued)

Check	Tester	Calibrated Points	Program	Seq	Control	Desired Results	Remarks
Output Amplitude and DC Offset (Continued)			Func ⎍ Freq 9.99E5 Ampl 1.00E0	40	A3C53, A3C56	Best square wave in both + and – amplitude	

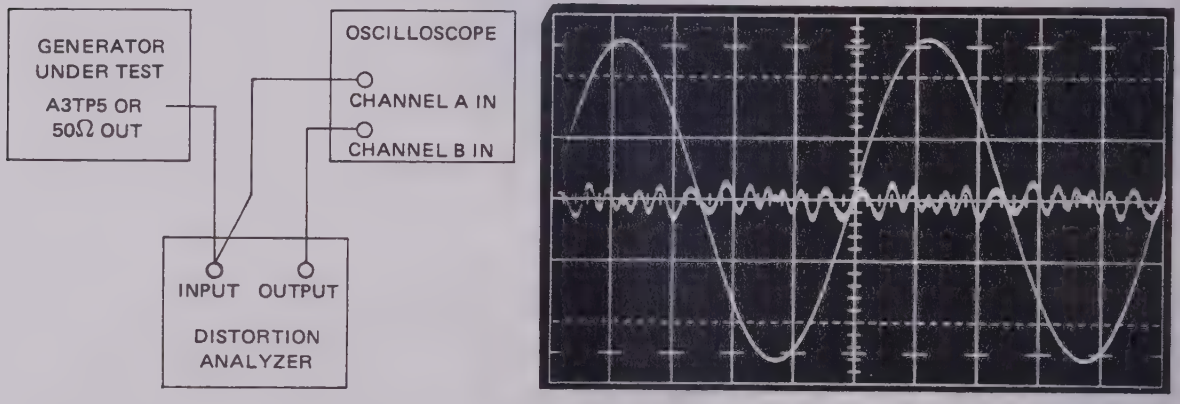

Figure 5-1. Distortion Analysis Test Setup

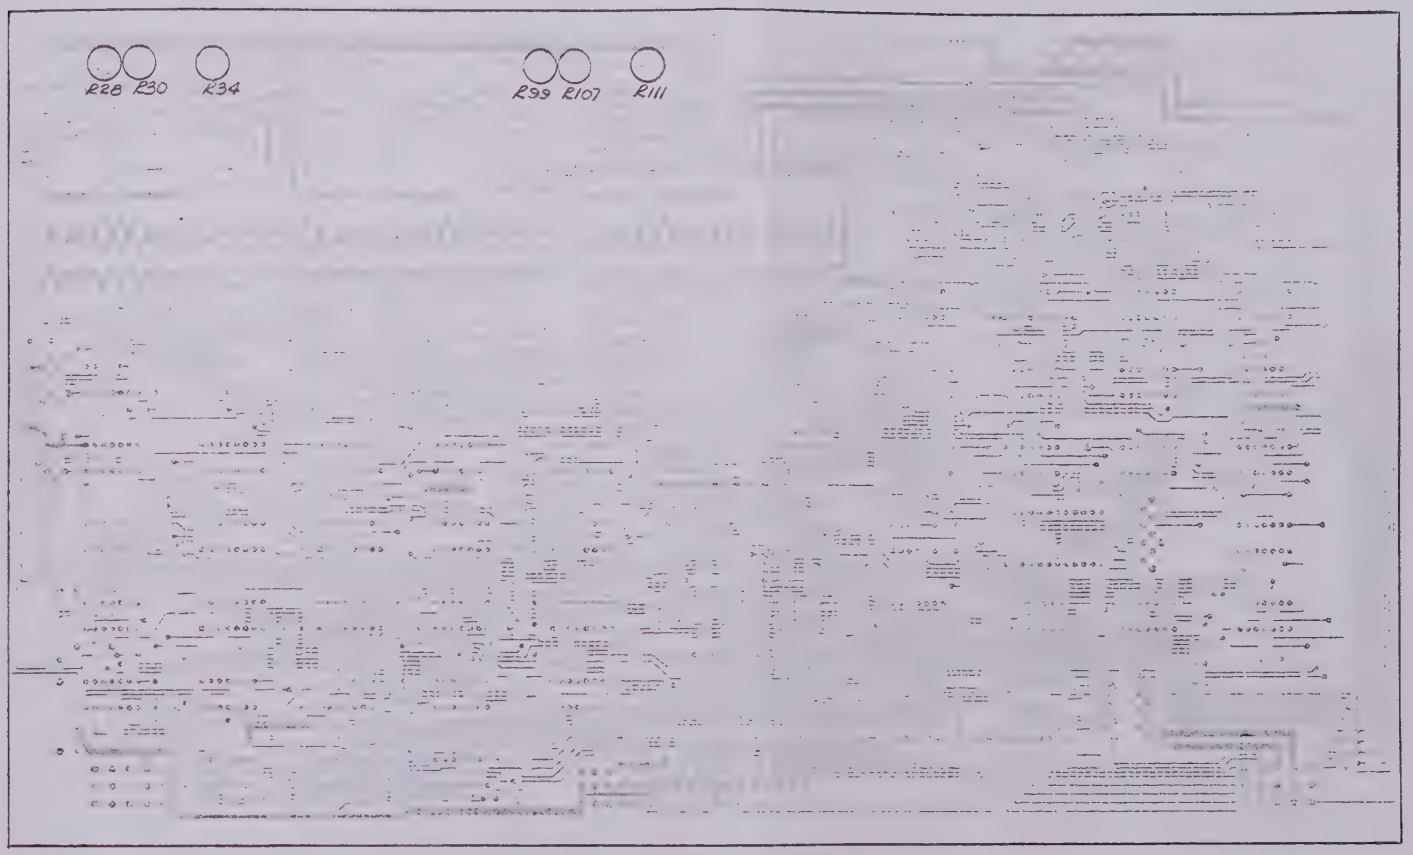

DIGITAL BOARD

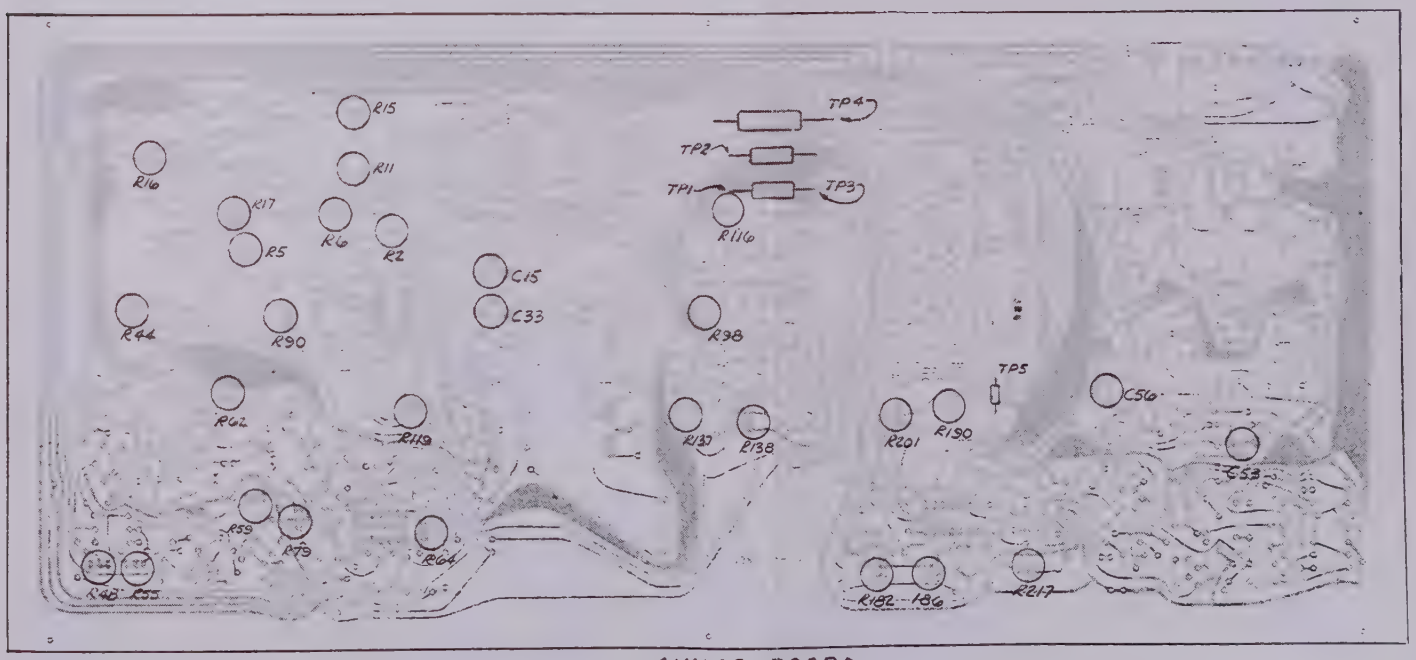

ANALOG BOARD

Figure 5-2. Calibration Drawing

SECTION 6
TROUBLESHOOTING

6.1 CORRECTIVE MAINTENANCE

This portion of the manual presents a systematic approach to troubleshooting. It is composed of three parts:

Part 1. Troubleshooting Techniques for Individual Components (Paragraph 6.2) — Frequently you can quickly locate a defective component by this technique without understanding the detailed function of the circuit. It is also a necessary technique when extensive troubleshooting in the component level is required.

Part 2. Quick Troubleshooting Guide (Paragraph 6.3) — Start by observing the symptoms of malfunctioning; then use the guide to find the defective components or malfunctioning circuits.

Part 3. Key Signals, Voltages and States (Table 6-1) — This is a supplemental procedure to Part 2 and used to locate defective components within the malfunctioning circuits.

6.2 TROUBLESHOOTING TECHNIQUES FOR INDIVIDUAL COMPONENTS

6.2.1 Bipolar Transistor

1. A transistor is defective if more than one volt (typically 0.7V) across the base/emitter junction is measured in the forward direction.
2. A transistor, when used as a switch, may have a few volts reverse bias voltage.

6.2.2 Diode

A diode is defective if it has greater than one volt (typically 0.7V) forward voltage across it (except Zener and LED).

6.2.3 Operational Amplifier (e.g., 741, CA3030)

The + and — inputs of an operational amplifier should have less than 15 mV difference when operating under normal conditions.

6.2.4 FET (Field Effect Transistor)

1. No gate current should be drawn by the gate. If so, the FET is defective.
2. The gate-to-source voltage is always reversed biased under normal operating conditions. If otherwise, the FET is defective.

6.2.5 Capacitor

1. Shorted capacitors have zero volts across their terminals.
2. Opened capacitor can be located (but not always) by using a good capacitor connected in parallel with the capacitor under test and observing the resulting effect.

6.3 QUICK TROUBLESHOOTING GUIDE

Symptom	Corrective Action
Blown Line Fuse	Replace fuse. If it blows again, check the following: 1. One of the four transistors mounted on the rear panel is shorted to itself or to chassis ground. 2. Bypass capacitors for power supply are shorted. 3. Follow algorithm (Figure 6-1) to locate short in a particular supply.

Symptom	Corrective Action
+15V Power Supply Malfunction	1. Voltage low: a. Transformer output low. b. Extra current loading; check for overheated and defective component. Use P1, P2 and P3 for isolation of current loading. 2. Voltage high: a. Power transistor Q1 and Q2 shorted. b. IC1 defective.
Other Power Supply Malfunctions	1. Use similar procedure for troubleshooting as in the +15V power supply malfunctions. 2. Follow Figure 6-1 to locate problem in a particular power supply.
No Output Signals	1. If no ∿ signal is present at output of integrator, follow Figure 6-2 for trouble-shooting. 2. If no signal is present at TP5, check function selector in Table 6-1. 3. If no signal is seen at junction of R243 and R245, follow Figure 6-3, output amplifier.
∿ but no ∿ , ⎍ or ⌐	Follow Table 6-1 to check out the corresponding circuit.
Frequency Accuracy Out of Specification	1. Check frequency calibration. 2. Check for frequency change when changing frequency bit-by-bit; if problem appears to be in frequency setting, check D/A circuitry.
Amplitude Accuracy Out of Specification	1. Check calibration. 2. Check for amplitude change when changing amplitude bit-by-bit; if problem appears to be in amplitude setting, check D/A circuitry. 3. Check for saturation of output amplifier (50Ω loaded; amplitude plus dc offset should not exceed 10V p-p).
DC Offset Accuracy Out of Specification	1. Check calibration. 2. Check for offset change when changing offset bit-by-bit; if problem appears to be in offset setting, check D/A circuitry.
TRIG and GATED Mode Inoperative	1. Check for correct signals in the trigger circuit using Table 6-1.

Table 6-1. KEY SIGNALS, VOLTAGES AND STATES AT THE ANALOG BOARD

Frequency Range Logic

FR2	FR1	FR0	IC6 Pin In Low State	Frequency Range (Ex = X 10^X)
L	L	L	10	E0
L	L	H	11	E1
L	H	L	12	E2
L	H	H	13	E3
H	L	L	4	E4
H	L	H	3	E5
H	H	L	2	E6
H	H	H	1	E7

Generator Enable Circuit (Analog Board)

	Continuous	Trig/Gated (No Ext Trigger)
1. P3 pin 31 (OPERATE)	Low State	High State
2. Q14 base	0V	≈ 0.7V

Integrator

1. IC9 pin 4	≈ 0V
2. IC9 pin 5	≈ 1.4V
3. IC11 pin 12	≈ 2.5V p-p ∿
4. R135 & R136 junction	2.5V p-p ∿

Comparator Switch

1. Q2 & Q6 emitters	≈ +9V
2. IC7 pins 2 & 8	≈ −1V
3. Q2 base	≈ +8V with 0.5V p-p ⎍
4. Q6 base	≈ +8V with 0.5V p-p ⎍ opposite phase of Q2 base
5. Q1 emitter	≈ +2V/−1.5V ⎍
6. Q7 emitter	≈ +2V/−2.5V ⎍

Ramp Amplifier

1. Q8 & Q12 emitters	+0.7V/−2V ⎍
2. IC8 pin 1	≈ +11V
3. IC8 pins 3 & 11	≈ −3V with ≈ 0.5V p-p ⎍ opposite phase from pin 3 to pin 11
4. IC8 pin 6	+1.25V
5. IC8 pin 2	2.5V p-p ∿
6. Q9 emitter	2.5V p-p ⌇

VCG

Voltages depend upon frequency setting.

1. P3 pin 46 (D/F)	0 to −10V
2. IC1 pin 6	0 to +3.7V
3. Q3 emitter	−0.7V to −4.0V
4. IC3 pin 6	+0.7V to +4.0V

Sine Converter and Amplifier

1. IC12 pin 6	≈ 1.2 mV p-p ∿
2. IC10 pin 4	≈ 250 mV p-p ∿
3. IC10 pin 12	2.5V p-p ∿

Function Selector

$\overline{F0}$	$\overline{F1}$	Function	Collector of Q43	Q18	Q19	Q20
H	H	∿	≈ +5V	≈ −14V	≈ −14V	≈ −14V
H	L	∿	≈ −14V	≈ +5V	≈ −14V	≈ −14V
L	H	⎍	≈ −14V	≈ −14V	≈ +5V	≈ −14V
L	L	◿	≈ −14V	≈ −14V	≈ −14V	≈ +5V

X-Y Multiplier, Inverting Amplifier and Output Amplifier

1. P3 pin 7 (D/V)	−2V to +2V depending on amplitude setting and polarity
2. IC17 pin 4	Selected ∿ , ∿ , ⎍ or ⌇
3. IC17 pins 3 & 13	≈ −13V
4. IC17 pin 1	≈ 6V
5. IC17 pins 2 & 14	≈ 11V with low level amplitude of selected function
6. Q27 emitter	≈ −4V
7. Q21 base	≈ +13V
8. Q22 base	≈ −13V
9. Q28 emitter	≈ +6V
10. Q32 emitter	≈ +6V
11. Q33 base	≈ +13V
12. Q34 base	≈ −13V
13. Q37 & Q38 collectors	≈ twice programmed amplitude p-p
14. R243 & R245 junction	≈ twice programmed amplitude p-p
15. Q21, Q22, Q27 thru Q38, Q41 & Q42	On in any normal state (i.e., base/emitter drop should be ≈ 0.7V in forward bias direction)
16. Q39 & Q40	On only when output sinks or sources >100 mA

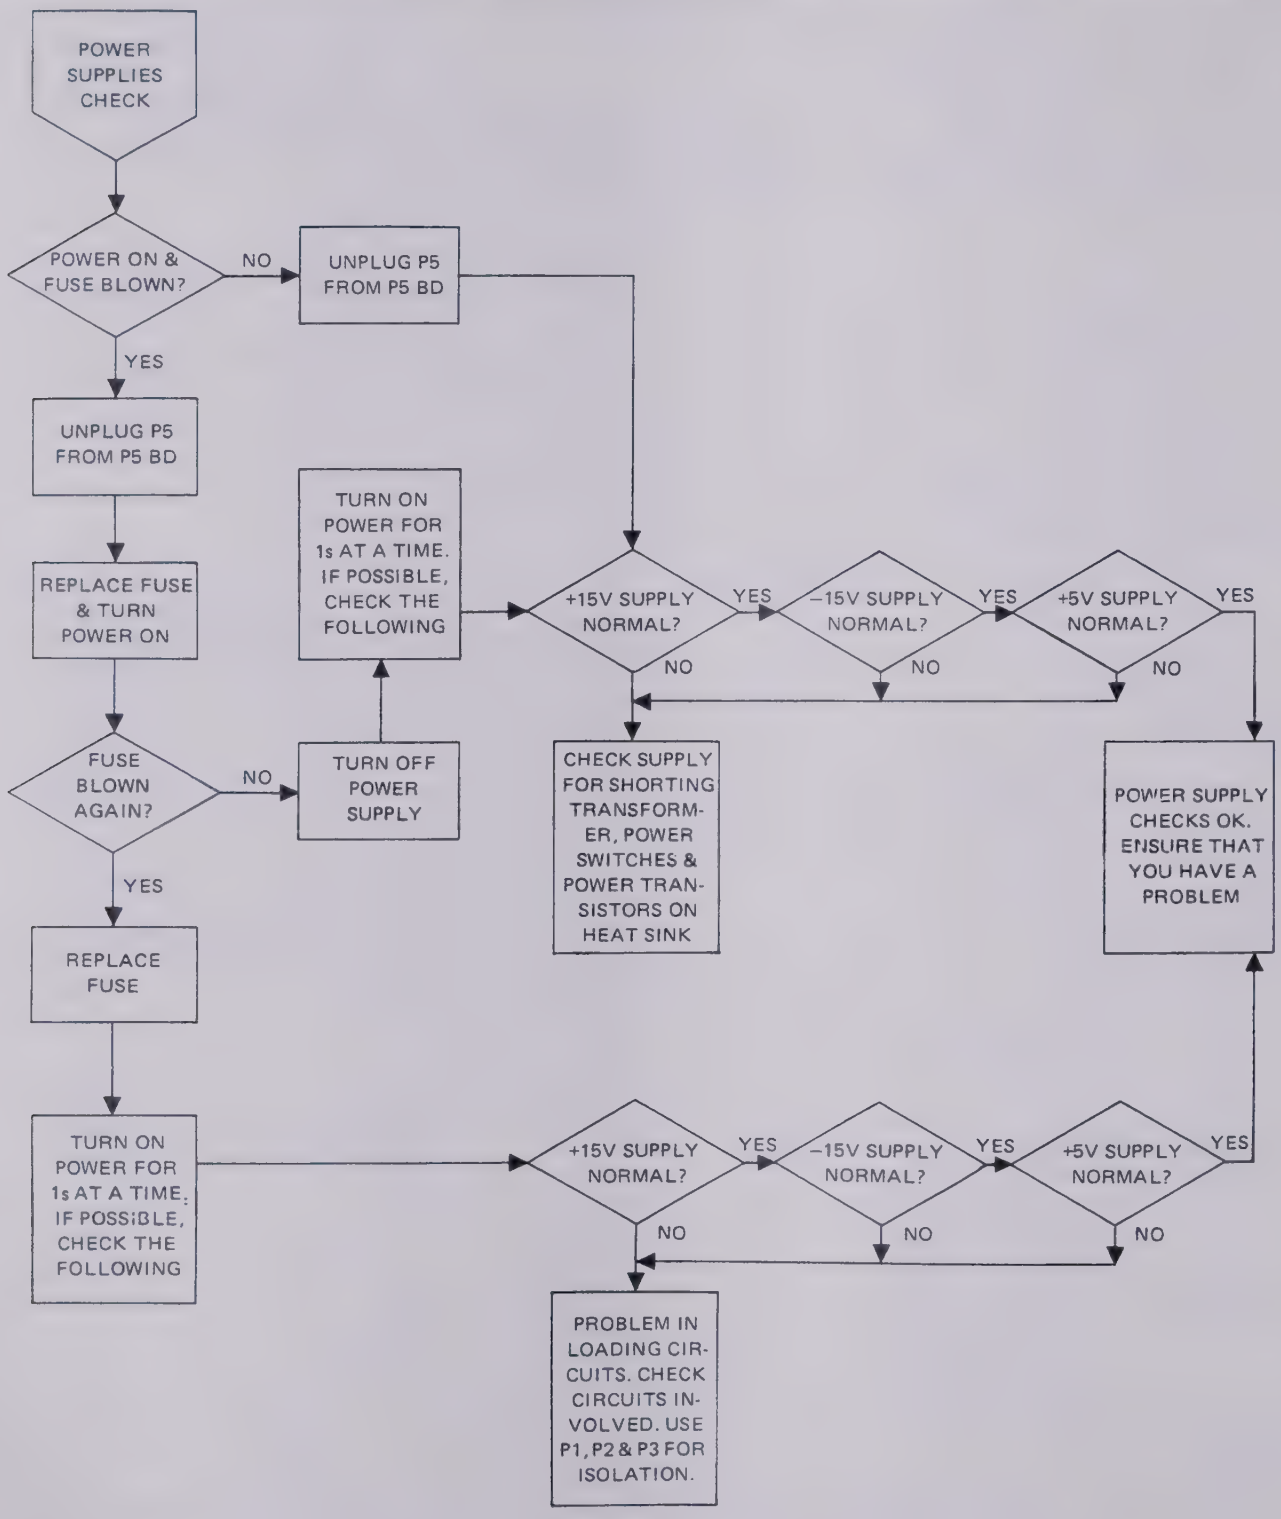

Figure 6-1. Power Supply Algorithm

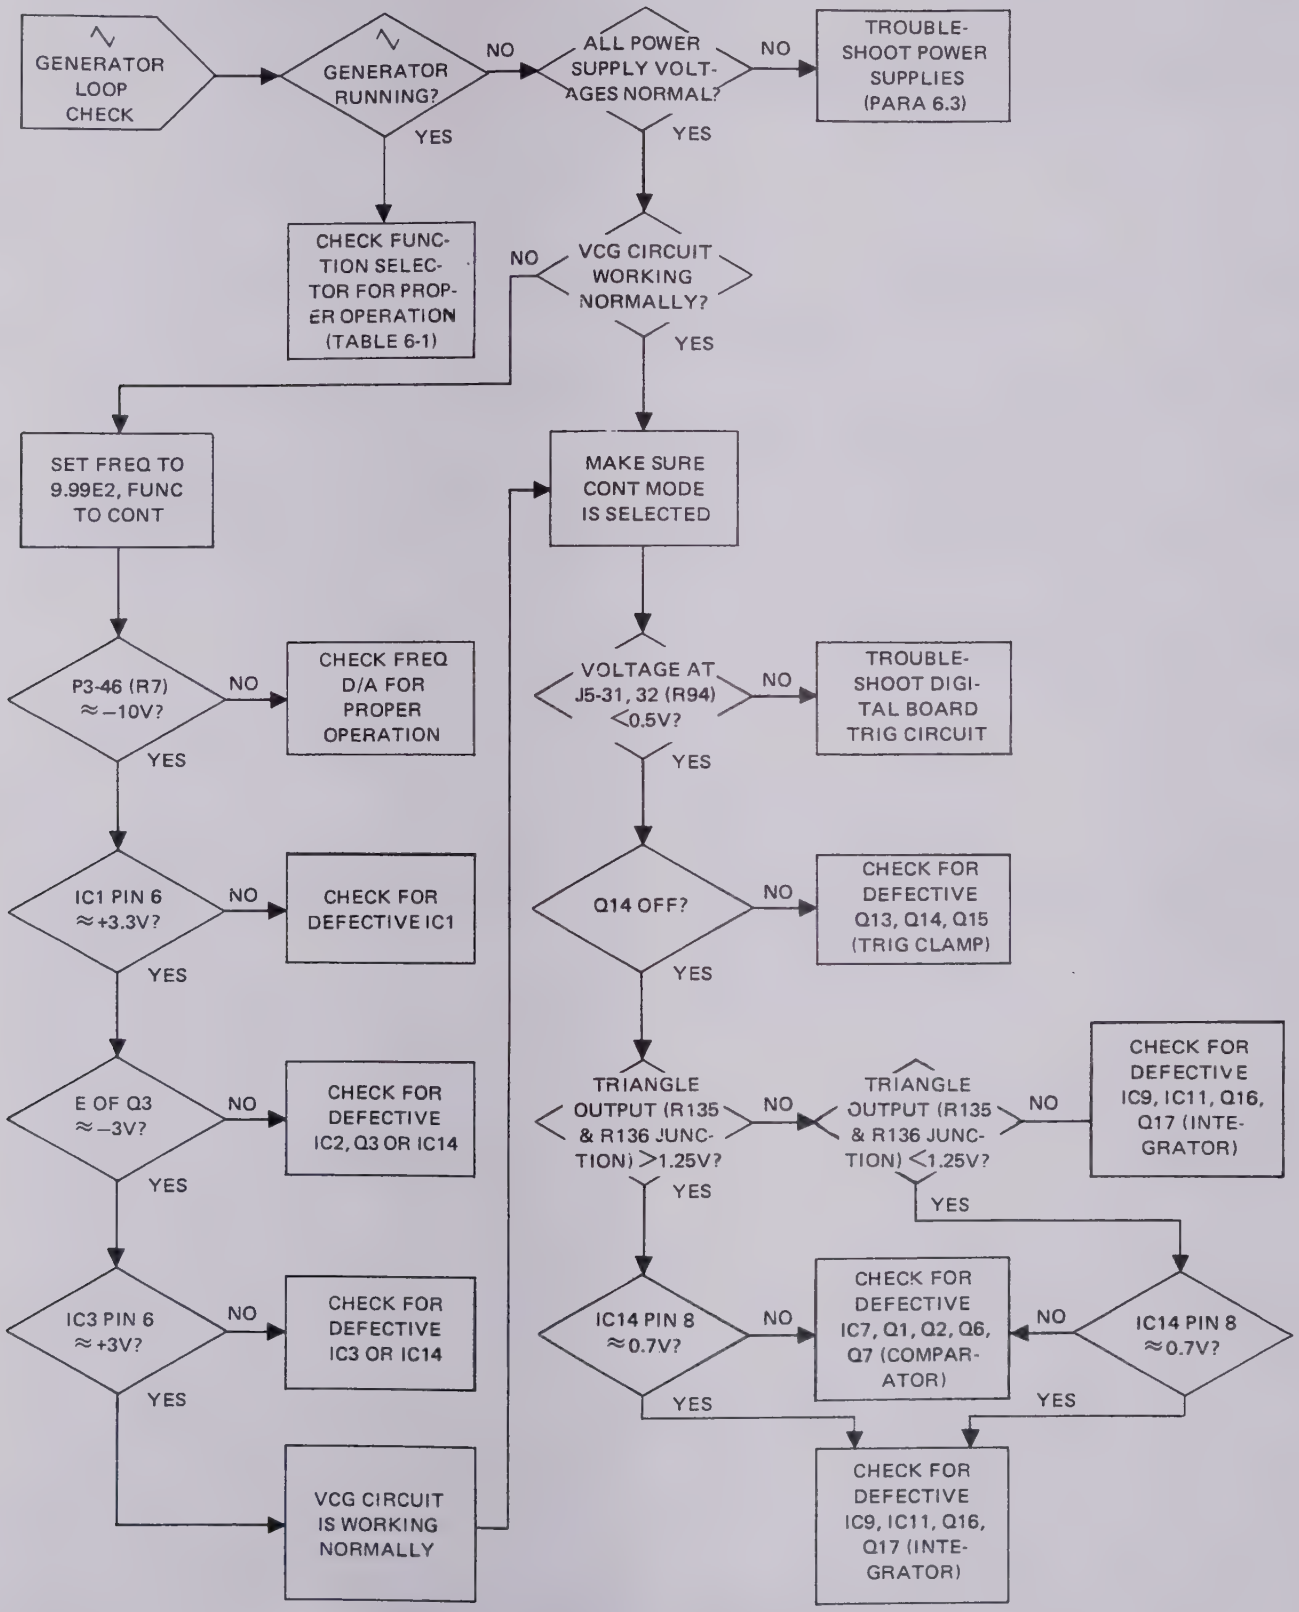

Figure 6-2. Integrator, Comparator and VCG Algorithm

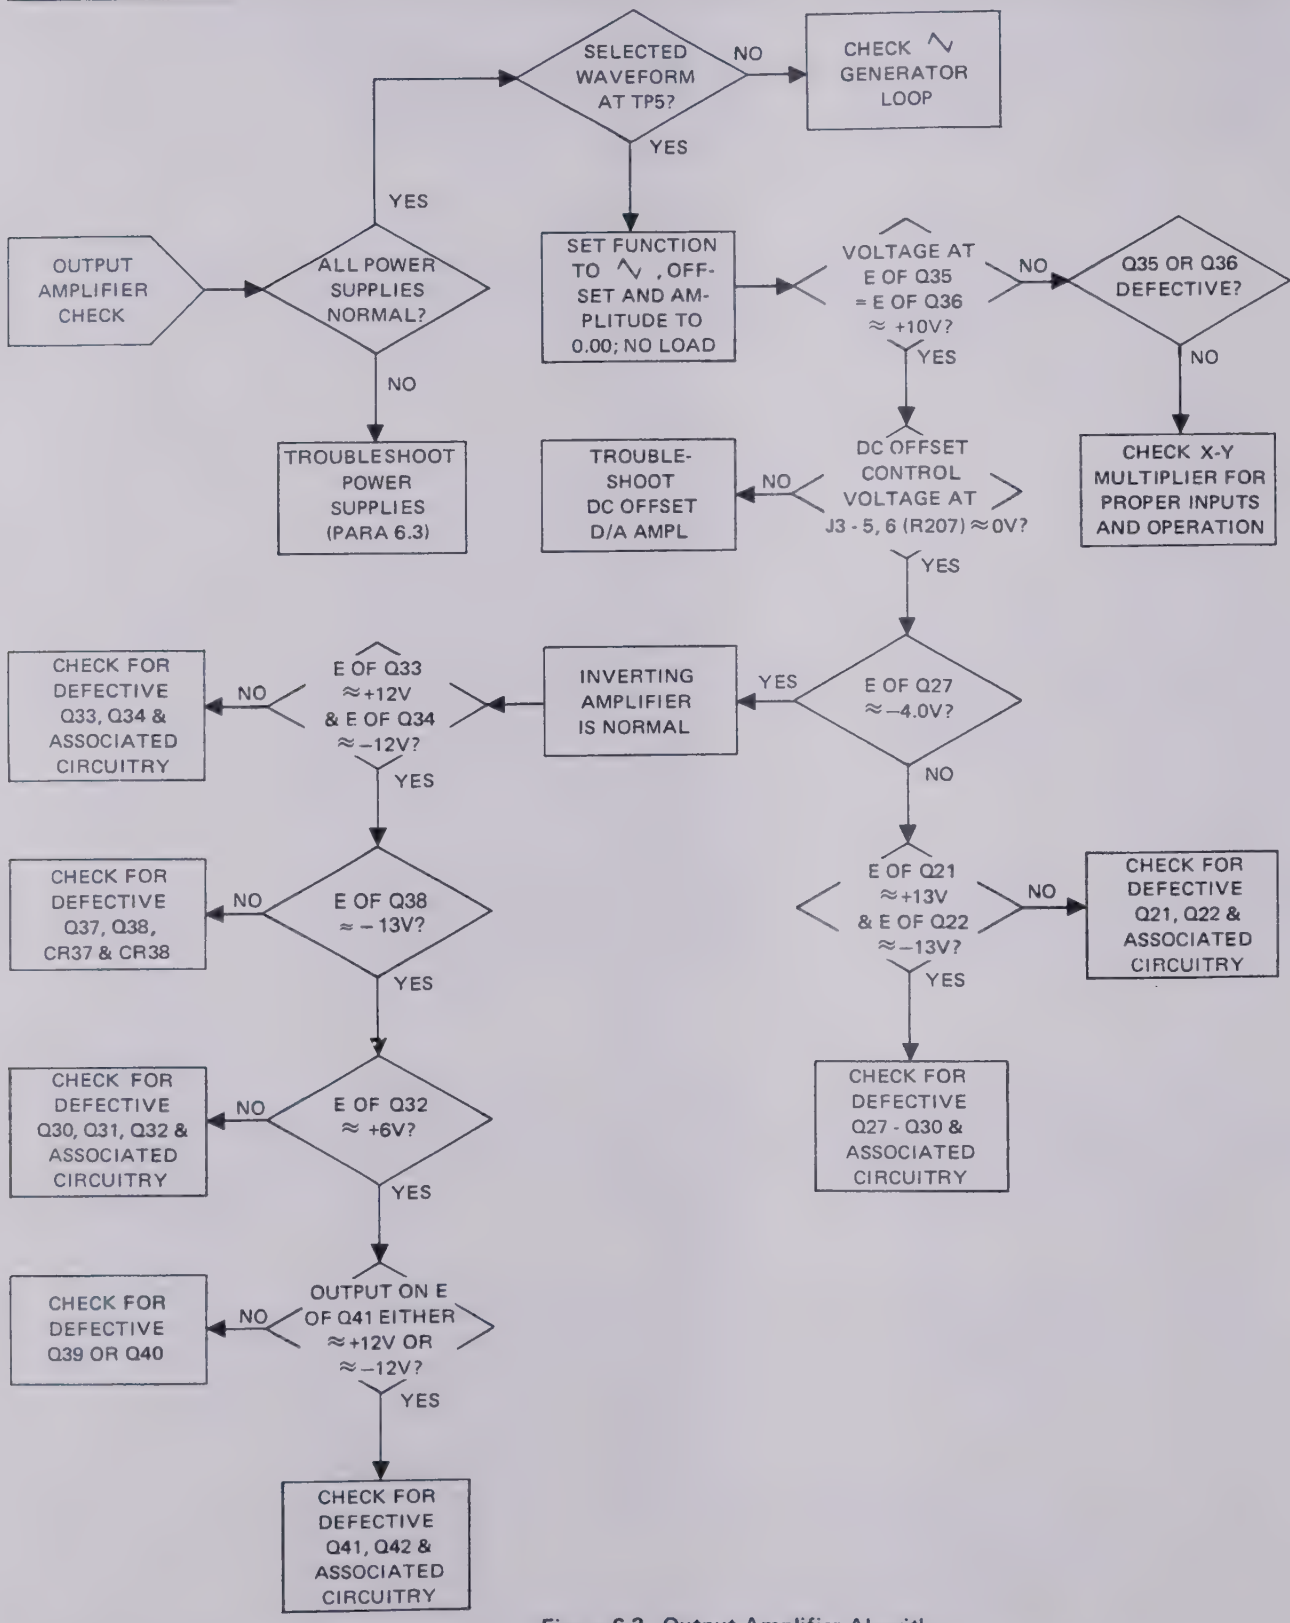
SELECTED WAVEFORM AT TP5?
NO
CHECK ∿ GENERATOR LOOP
YES
OUTPUT AMPLIFIER CHECK
ALL POWER SUPPLIES NORMAL?
YES
NO
TROUBLESHOOT POWER SUPPLIES (PARA 6.3)
SET FUNCTION TO ∿, OFFSET AND AMPLITUDE TO 0.00; NO LOAD
VOLTAGE AT E OF Q35 = E OF Q36 ≈ +10V?
NO
Q35 OR Q36 DEFECTIVE?
YES
NO
CHECK X-Y MULTIPLIER FOR PROPER INPUTS AND OPERATION
TROUBLE-SHOOT DC OFFSET D/A AMPL
NO
DC OFFSET CONTROL VOLTAGE AT J3 - 5, 6 (R207) ≈0V?
YES
CHECK FOR DEFECTIVE Q33, Q34 & ASSOCIATED CIRCUITRY
NO
E OF Q33 ≈+12V & E OF Q34 ≈–12V?
INVERTING AMPLIFIER IS NORMAL
YES
E OF Q27 ≈–4.0V?
YES
NO
CHECK FOR DEFECTIVE Q37, Q38, CR37 & CR38
NO
E OF Q38 ≈ – 13V?
YES
E OF Q21 ≈+13V & E OF Q22 ≈–13V?
NO
CHECK FOR DEFECTIVE Q21, Q22 & ASSOCIATED CIRCUITRY
YES
CHECK FOR DEFECTIVE Q30, Q31, Q32 & ASSOCIATED CIRCUITRY
NO
E OF Q32 ≈ +6V?
YES
CHECK FOR DEFECTIVE Q27 - Q30 & ASSOCIATED CIRCUITRY
CHECK FOR DEFECTIVE Q39 OR Q40
NO
OUTPUT ON E OF Q41 EITHER ≈+12V OR ≈–12V?
YES
CHECK FOR DEFECTIVE Q41, Q42 & ASSOCIATED CIRCUITRY

Figure 6-3. Output Amplifier Algorithm

SECTION 7
PARTS AND SCHEMATICS

7.1 DRAWINGS

The following assembly drawings (with parts lists) and schematics are in the arrangement shown below.

7.2 ORDERING PARTS

When ordering spare parts, please specify part number, circuit reference, board, serial number of unit, and, if applicable, the function performed.

Drawings	Old Number	New Number
Instrument Schematic	158-200	0004-00-0045
Chassis Assembly	159-000	0102-00-0304
Chassis Parts List	159-000	1101-00-0045
Display Board Schematic	158-218	0103-00-0105
Display Board Assembly	158-018	0101-00-0105
Display Board Parts List	158-018	1100-00-0105
Analog Board Schematic	158-219	0103-00-0107
Analog Board Assembly	158-019	0101-00-0107
Analog Board Parts List	158-019	1101-00-0107
Front Panel Assembly	159-046	0102-00-0333
Front Panel Parts List	159-046	1101-00-0075
Key Board Schematic	158-247	0103-00-019
Key Board Assembly	158-047	0101-00-0109
Key Board Parts List	158-047	1100-00-0109
Display Board Schematic	158-251	0103-00-0105
Display Board Assembly	158-051	0101-00-0105
Display Board Parts List	158-051	1100-00-0105
Rear Panel Assembly	158-034	0102-00-0332
Rear Panel Parts List	158-034	1101-00-0074
Power Supply Schematic	158-220	0103-00-0108
Power Supply Assembly	158-020	0101-00-0108
Power Supply Parts List	158-202	1100-00-0108
158 Instrument Schematic	158-235	0004-00-0081
158 Modification	158-000	0102-00-0303
158 Modification Parts List	158-000	1101-00-0044
158 Front Panel Assembly	158-038	0102-00-0336
158 Front Panel Parts List	158-038	1101-00-0078
158 Cable Assembly	158-039	1203-00-0005

7.3 ADDENDA

Under Wavetek's product improvement program, the latest electronic designs and circuits are incorporated into each Wavetek instrument as quickly as development and testing permit. Because of the time needed to compose and print instruction manuals, it is not always possible to include the most recent changes in the initial printing. Whenever this occurs, addendum pages are prepared to summarize the changes made and are inserted immediately inside the rear cover. If no such pages exist, the manual is correct as printed.

Drawings	Number
005 Interconnect Diagram	0040-00-0080
GPIB Interface Schematic	0103-00-0972
GPIB Interface Assembly	0101-00-0972
GPIB Interface Parts List	1100-00-0972
005 Modification Drawing	0102-00-0351
005 Modification Parts List	1101-00-0229
005 Cable Assembly	1207-00-0004
005 ASCII I/O Cable Assembly	1203-00-0003

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE
A	ECN 1133	DO	11/3/6
B	ECN 1368	DO	11-17-75
C	# 1920	Ervin Sellowitz	5-7-79

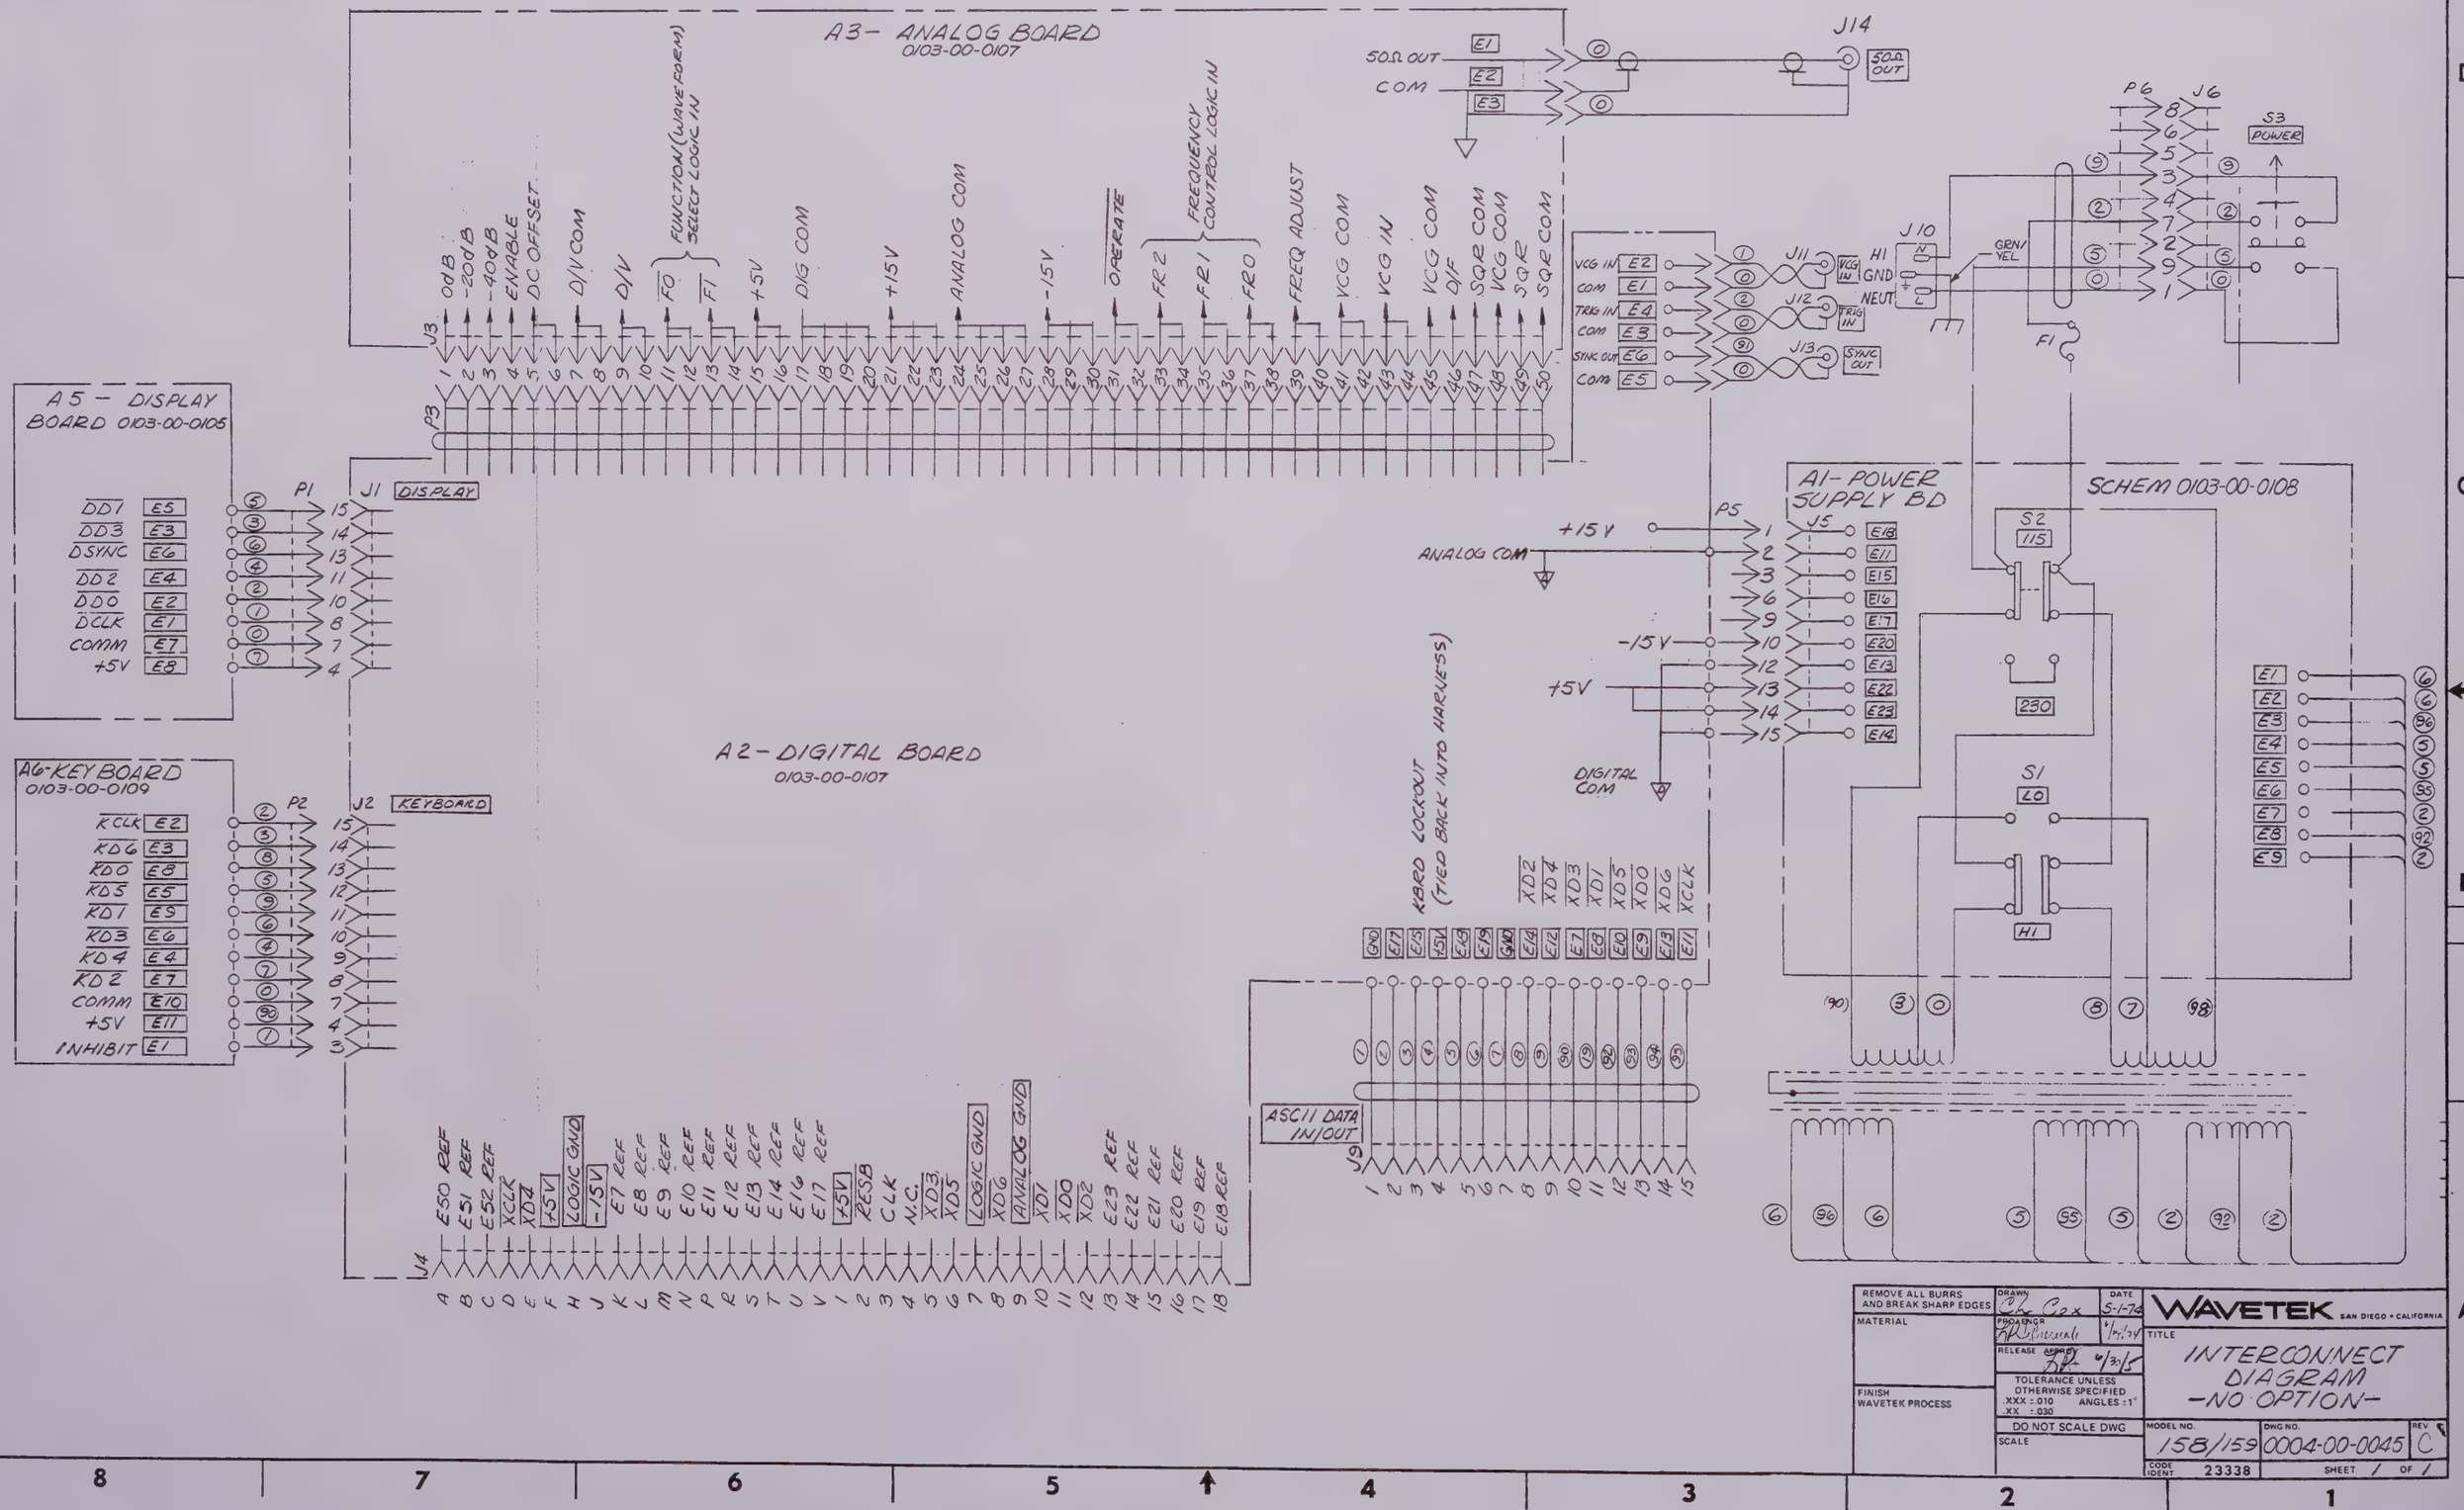

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN PL Cox	DATE 5-1-74	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR [illegible]	6/17/74	TITLE: INTERCONNECT DIAGRAM -NO OPTION-
FINISH WAVETEK PROCESS	RELEASE APPROVED [illegible]	6/3/75	
	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030		
	DO NOT SCALE DWG		MODEL NO. 158/159
	SCALE		DWG NO. 0004-00-0045 REV C
			CODE IDENT 23338 SHEET 1 OF 1

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	1069	CL	8/20	LB
B	ECN 1125	RO	11/30/76	LPS
C	1196	RO	1/24/78	LPS
D	ECN 1754	RO	6-27-78	LPS
/	ECN 3750	DC	5-10-83	LPS
E	3933	SC	9-19-83	LPS

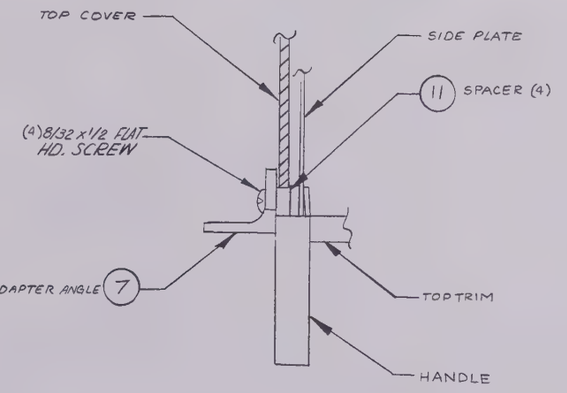

DETAIL A



DETAIL B

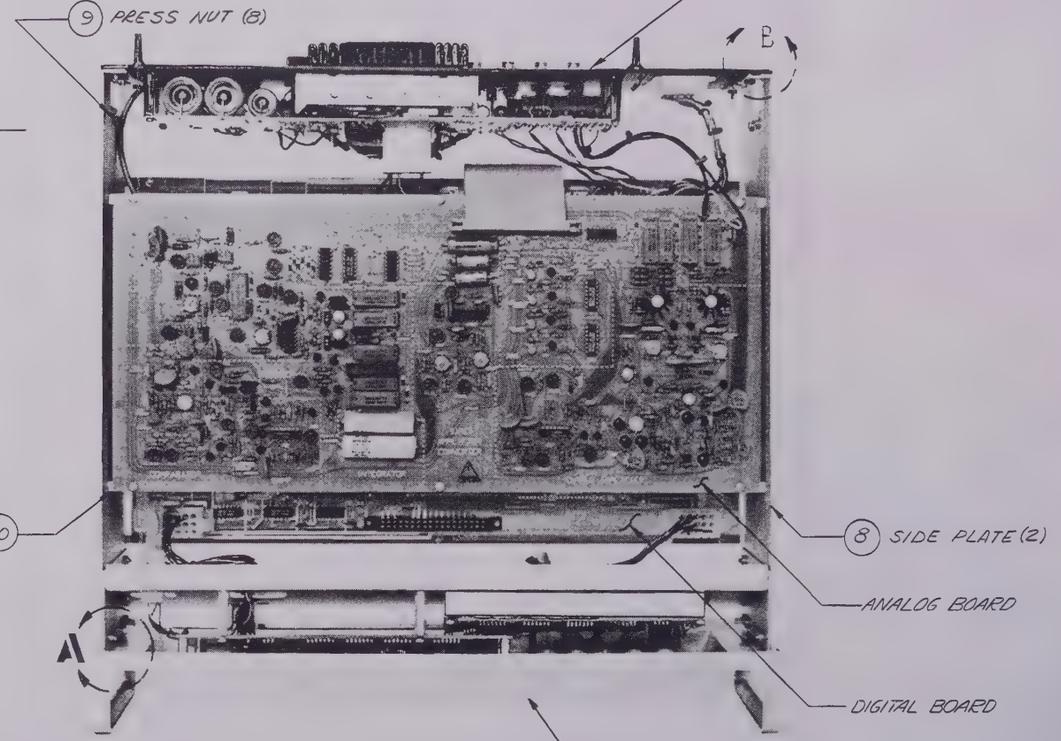

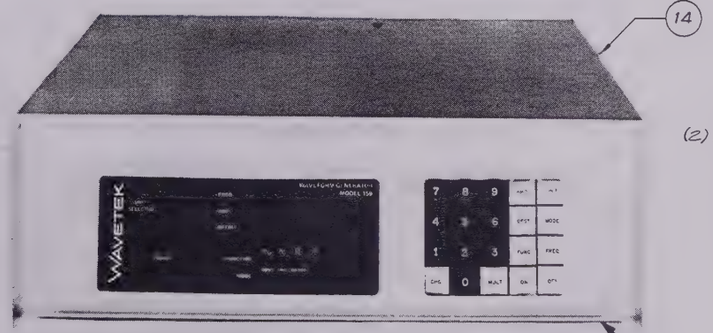

TOP VIEW WITH COVERS REMOVED

1. ITEM 6&7 ARE NOT SHOWN.

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN C.L. Cox	DATE 5/24/76	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL —	PROJ ENGR L.P. Simmons	6/24/76	TITLE ASSEMBLY CHASSIS
FINISH WAVETEK PROCESS —	RELEASED / IMPROV LPS	12/14/79	
	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ± .010 ANGLES ±1 XX ± .030		
	DO NOT SCALE DWG		MODEL NO 159
	SCALE NONE		DWG NO 0102-00-0304 REV E
			CODE IDENT 23338 SHEET 1 OF 2

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	ASSY DRWG, CHASSIS	0102-00-0304	WVTK	0102-00-0304	1
5	ASSY, COVER	1201-00-1163	WVTK	1201-00-1163	1
8	PLATE, SIDE	158-310	WVTK	1400-00-0673	2
14	COVER, TOP FROM: 1400-00-9020	158-341	WVTK	1400-00-0779	1
7	BRKT, ANGLE, R/A	146-373-PAINT	WVTK	1400-00-2712	2
11	SPACER, R/A	147-362	WVTK	1400-00-3693	4
12	BAIL W/FEET, 15 1/2	BAIL 15 1/2	BUKEY	2800-08-0001	1
13	SPEEDNUT, SELF RETAIN	C7494-632-4	TINN	2800-09-0003	6
9	INSERT # 6	74-11-106-13	SOTCO	2800-09-0017	8
10	FAST, CHASSIS	1591-C11	USECO	2300-09-0022	2
NONE	PWR CORD	6001-80-0005	WVTK	6001-80-0005	1

WAVETEK PARTS LIST

TITLE
STD CHASSIS

ASSEMBLY NO.
1101-00-0045

PAGE: 1

REV
E

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: PARTS LIST STD CHASSIS
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030		
	DO NOT SCALE DWG		MODEL NO. 159 / DWG NO. 1100-00-0045 / REV E
	SCALE		CODE IDENT 23338 / SHEET 1 OF 1

B:SHOP GRAPHICS/ACCUPRESS
REORDER NO. A-3894

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	ECN 3160	DC	3/30/82	
/	ECN 3404 CL III	DC	11/2/82	
B	3442		11/18/82	
/	3480		12/3/82	
/	3796 (CL II		6/1/83	

OPTIONAL INTERFACE CONVERSION PCA

OPTIONS ONLY: U V 18 17 T R K L N M S P

2 3 4

OPTIONS ONLY: 16 15 14 13

J -15V

9 1 7 H F C B A

OPTIONS ONLY

ANALOG COMM, +5V, DIG COMM, DIG COMM

XCLK (OPT OUT), XD6 (OPT OUT), XD0 (OPT OUT), XD5 (OPT OUT), XD1 (OPT OUT), XD3 (OPT OUT), XD4 (OPT OUT), XD2 (OPT OUT)

D 8 11 6 10 5 E 12

INTERFACE CONNECTOR J4

(287) ESB, (347) CLK, N.C.

E20 E21 E22 E23 -15V +5V +5V +5V E32 E31 E30

CONTROL	ASCII	D6	D5	D4	D3	D2	D1	D0
CHS	–	L	H	H	H	H	L	H
0	0	L	H	H	L	L	L	L
1	1	L	H	H	L	L	L	H
2	2	L	H	H	L	L	H	L
3	3	L	H	H	L	L	H	H
4	4	L	H	H	L	H	L	L
5	5	L	H	H	L	H	L	H
6	6	L	H	H	L	H	H	L
7	7	L	H	H	L	H	H	H
8	8	L	H	H	H	L	L	L
9	9	L	H	H	H	L	L	H
AMPL	A	H	L	L	L	L	L	H
MODE	B	H	L	L	L	L	H	L
FUNC	C	H	L	L	L	L	H	H
OFST	D	H	L	L	L	H	L	L
MULT	E	H	L	L	L	H	L	H
MULT (NOTE)	SP	L		L	L	L	L	L
FREQ	F	H	L	L	L	H	H	L
UNIT	G	H	L	L	L	H	H	H
ON	H	H	L	L	H	L	L	L
OFF	I	H	L	L	H	L	L	H

NOTE: USE OF ASCII "SPACE" (SP) ENABLED ONLY BY AN IMMEDIATELY PRECEDING NUMERAL

OPERATION	CONTROLS
CONT	MODE 0
TRIG	MODE 1
GATE	MODE 2
∿	FUNC 0
⩘	FUNC 1
⎍	FUNC 2
⩙	FUNC 3

CLK =	$\overline{KCLK}$	OR	$\overline{XCLK}$
D0 =	$\overline{KD0}$	OR	$\overline{XD0}$
D1 =	$\overline{KD1}$	OR	$\overline{XD1}$
D2 =	$\overline{KD2}$	OR	$\overline{XD2}$
D3 =	$\overline{KD3}$	OR	$\overline{XD3}$
D4 =	$\overline{KD4}$	OR	$\overline{XD4}$
D5 =	$\overline{KD5}$	OR	$\overline{XD5}$
D6 =	$\overline{KD6}$	OR	$\overline{XD6}$

DATA BIT (KEYBOARD) FROM J2 (REMOTE) FROM J7

J9

+5V, GND

E16 E17 E15 +5V E18 E19 E40 E14 E12 E7 E8 E10 E9 E13 E11

STANDARD INTERFACE ENABLE STRAPS (REMOVED IN OPTIONS)

E49	$\overline{XD2}$	E48	
E45	$\overline{XD4}$	E44	
E35	$\overline{XD3}$	E34	
E37	$\overline{XD1}$	E36	
E41	$\overline{XD5}$	E40	
E39	$\overline{XD0}$	E38	
E47	$\overline{XD6}$	E46	
E43	$\overline{XCLK}$	E42	

74132 IC42 B → D2 (2D8, 2B8)

IC34 D → D4 (2C8)

IC42 C → D3 (2C8, 2B8)

IC42 D → D1 (2C8, 2D8, 2D2)

IC34 B → D5 (2C8)

IC42 A → D0 (2D8, 2C8, 2D2, 2B5)

IC34 C → D6 (2C8)

IC34 A 74132 → CLK (2C8)

KEYBOARD J2

N.C. 1, N.C. 2, KEYBOARD INHIBIT 3, +5V 4, N.C. 5, N.C. 6, COM 7, $\overline{KD2}$ 8, $\overline{KD4}$ 9, $\overline{KD3}$ 10, $\overline{KD1}$ 11, $\overline{KD5}$ 12, $\overline{KD0}$ 13, $\overline{KD6}$ 14, $\overline{KCLK}$ 15

TERMINATION SOCKET XIC41

IC 41 R220/330

TERMINATION PACK (ONE PER MULTI-UNIT GROUP)

+5V → 14; 8 3 9 5 1 6 4 2 7

+5V (C) (G) (L) (A) (J) (Q) (E) (N) — 220Ω

(D) (H) (M) (B) (K) (R) (F) (P) — 330Ω

6. NOTE: ** NOM VALUE CALLED OUT ON P/L

5 CONNECTOR FOR "ASCII DATA IN/OUT" OR "ISOLATED ASCII DATA IN" FOR APPROPRIATE PIN ASSIGNMENT SEE INTERCONNECT DIAGRAM.

4 BAR OVER MNEMONIC DENOTES TRUE-WHEN-LOW.

3. ○ DENOTES WIRE COLOR PER RESISTOR CODE.

2. ▭ DENOTES ACTUAL LABELING ON BOARD.

1. =▷* DENOTES OPEN COLLECTOR.

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES

MATERIAL

FINISH WAVETEK PROCESS

DRAWN C.L. Cox 5/15/74

PROJ ENGR 6/1/74

RELEASE APPROV

TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030

DO NOT SCALE DWG

SCALE

WAVETEK SAN DIEGO • CALIFORNIA

TITLE: SCHEMATIC A2 DIGITAL BOARD INTERFACE BUS)

MODEL NO. 158/159

DWG NO. 0103-00-0819

REV B

CODE IDENT 23338

SHEET 1 OF 6

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

BINARY-TO-HEXADECIMAL CONVERSION LOGIC

IC43 74154

(1B2) D0
(1C1) D1
(1C3) D2
(1C2) D3
ENBL

(1C2) D4
(1C1) D5
(1B2) D6
(1B3) CLK
ENABLE
IC35 74LS138

TRIG IN
E4
TRIG (B5)
ON REAR PANEL

CHS (ASCII) (C7) $\overline{20}$ (C7) $\overline{D}$
IC44 B 7402
MCLK (5B7, D5)
MINUS SIGN CLOCK (MCLK)

MINUS SIGN ENABLE (MSIGN) LOGIC
+3.7V
MCLK (D6)
IC45 7404
IC51B 7474
$\overline{40}$ (C7)
MSIGN (4A3, 5B7)

UNIT ENABLE (ITSME) LOGIC
E24 E29
(D7)
E25 E26 E27 E28 E30 E31 E32 E33
(C7) $\overline{30}$
7404 IC45
RESB
UNIT (ASCII G) (D7) $\overline{7}$ (C7) $\overline{40}$
IC46 B 7474
IC52 A
IC46 A 7474
ITSME (3B4, 3D3)
RESB

NUMERALS CLOCK (30C) LOGIC
IC31 A
$\overline{30}$ (C7)
30C (5B6, B6, C4, C2)

ON/OFF CONTROL (ENABLE)
ON (ASCII H)
OFF (ASCII I)
C4
IC45 IC55 B
(D7) $\overline{8}$ 40EC (D7) $\overline{9}$
7404 IC45 74107
ENABLE (C1)
$\overline{\text{ENABLE}}$ (3B4)
RESB

DISPLAY DIGITS RESET (ADRSET) R136 10K +5V
C7 33PF
(100MS)
IC56 9601
FUNC ASCII C
(D7) $\overline{3}$ (C4) $\overline{40C}$
ADRSET (4B6, 5B6 GA7)
N.C.

FUNCTION SELECT

FUNC	D0	D1	F0	$\overline{F0}$	F1	$\overline{F1}$
~	L	L	L	H	L	H
~	H	L	H	L	L	H
⊓	L	H	L	H	H	L
⊓	H	H	H	L	H	L

(1B2) D0
(1C1) D1
IC57B 74107
F0 (3B4)
RESB
IC54 A
IC49 B
IC57A 7474
F1 (4A2, 3B4)
TO ANALOG BOARD DWG 0103-00-0107
P3
$\overline{F0}$
$\overline{F1}$
30C (C4)

NUMERALS ENABLE LOGIC
(C4) $\overline{40EC}$
(C4) 30C
IC54 B 7474
IC49 A

SPACE-AS-MULT GATE
(ASCII SPACE)
(C7) $\overline{20}$ (D7) $\overline{0}$
IC44 C 7402
IC58 A 7408
IC44 A 7402
RNG CLK (4A7, 6A8)
(C7) $\overline{40}$ (D7) $\overline{5}$
MULT (ASCII E)
IC44 D 7402
RANGE (X10 MULTIPLIER) CLOCK (RNG CLK)

D3 4 ENABLE
(B8) VCG IN
+15V +15V
$\overline{\text{OPERATE}}$
+5V +5V
DIGITAL COM
ANALOG COM
-15V -15V
VCG COM

ALPHA (EXCEPT MULT) CLOCK (40EC)
MULT (ASCII E) (D7) $\overline{5}$ (C7) $\overline{40}$
IC33 B
IC53 A
IC53 D
IC45 B 7404
TP
40EC (4B7, 5B7, 6B5, B6, C4, D2)
40EC (4B7, 4B3 D4)

MANUAL TRIGGER
(B6) $\overline{\text{TRIGC}}$
(1B2) D0
7404 IC45
7437 IC52 B

GENERATOR ENABLE
+3.7V IC40A 74107
IC58 B
IC40B 74107
TRIG-MODE GATE IC47 B
ENABLE GATE IC52 C 7437
74132 IC47A GATE-MODE GATE
MO (TRIG)
M1 (GATE)
+15V R140 3.32K
R137 100
IC47 D 74132
7437 IC52 D
E6 E5
SYNC OUT
ON REAR PANEL

+5V R138 ** CR86 CR87 R139 1K 1W
-15V
74132 IC47C
SQUARING GATE
MO (3B4)
TRIG (C8)

2 STAR CONVERTER
(1B2) D0
(1C1) D1
(1C3) D2
(1C2) D3
IC48 C 7402
IC48 B
IC48 D
IC48 A
D0* (6A6, 6B4, 5B4, 4B4)
D1* (6A6, 6B4, 5B4, 4B4)
D2* (6A6, 5B4, 4B4)
D3* (6B4, 5B4, 4B4)
D0* = 2^0
D1* = 2^1
D2* = 2^2
D3* = 2^1

VCG IN
E2
(C1)
ON REAR PANEL

TURN-ON RESET (RESA, RESB)
R127 21.5K +5V
C31 33UF
IC1 E
IC2 9601
R128 2.21K +5V
IC53 B 7437
RESA (4B6, 4A5, 6B8)
RESB

TRIGGER CLOCK (TRIG)
MODE (ASCII B) (D7) $\overline{2}$ 40EC (C4)
RESB
IC12B 7474
IC49 D 7400
30C (C4)
$\overline{\text{TRIGC}}$ (B5)

MODE SELECT (M0, M1)

MODE	M0	M1
CONT	L	L
TRIG	H	L
GATE	L	H

RESB
IC50A 7474
IC50B 7474
(D7)
$\overline{2}$ (D7)
M0 (3B4)
M1 (3B4)
RESB

FROM ANALOG BD DWG 0103-00-0107
P3
SQR 49
SQR COM 50
TO PWR SUPPLY DWG 0103-00-0108
P5
+15V
ANALOG COM
-15V
DIGITAL COM
+5V
R135 2.21K
+3.7V(±1.3V)

+5V
C12 250UF 16V
C27 22UF 15V
C28 22UF 15V
C7 C13 C20 C21 C22 C23 C24 C32
01UF 50V
C14 C15 C16 C25 C26 C29 C30
33UF 10V
+15V C8 22UF 15V C9 .01UF 15V
-15V C10 22UF 15V C11 .01UF 50V

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN Ch. Cox	DATE 5/10/84	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL —	PROG ENGR		TITLE SCHEMATIC A2 DIGITAL BOARD (CONTROL LOGIC)
FINISH WAVETEK PROCESS —	RELEASE APPROV		
	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 .XX ±.030 ANGLES ±1°		
	DO NOT SCALE DWG		MODEL NO. 158/159 DWG NO. 0103-00-0819 REV B
	SCALE —		CODE IDENT 23338 SHEET 2 OF 6

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

MULTIPLEX LOGIC FOR DISPLAY BUS (DDO DD1 DD2 & DD3)

DISPLAY BOARD | T1 | T2 | T3 | T4 | T5 | T6 | T7 | T8 | T9 |

CLK

IC37 COUNT 7 8 9 10 11 12 13 14 15 7

2^0 { K0, $\overline{K0}$ }

2^1 { K1, $\overline{K1}$ }

2^2 { K2, $\overline{K2}$ }

2^3 K3

XSYNO (USED TO LOAD SHIFT REGISTERS)

$\overline{D\ CLK}$

LOGIC STATES MARKED WITH AN X LOAD THE FOLLOWING ITEMS ON LOGIC BUS (DDO, DD1 DD2, DD3)

- RANGE DIGIT
- MOST SIGNIFICANT DIGIT
- MIDDLE DIGIT
- LEAST SIGNIFICANT DIGIT
- DISPLAY MODE AND MINUS SIGNS
- FUNCTION (WAVEFORM)
- OPERATION MODE AND UNIT SELECT

SELECT FREQ, AMPL OR OFFSET DISPLAY

$\overline{SELF}$ (6B8) → IC29 D (7400) → SDO

$\overline{SELA}$ (4B6), $\overline{SDLDFF}$ (5B7) → IC33 A (7410) → $\overline{SDO}$

IC29 C (7400) → SD1

IC33 C (7410) → $\overline{SD1}$

+5V → C33 .01

CLOCK

$\overline{CLK}$ (C2) → C300 470 pF

+5V → R133 49.9K, R134 301K → IC36 NE 555 TIMER

C19 470 pF, C18 .01μF 20V

MULTIPLEX TIME CODE

IC32 7404 (3.7V)

IC37 74161 BINARY COUNTER: 2^0 2^1 2^2 2^3; CARRY, $Q2^0$, $Q2^1$, $Q2^2$, $Q2^3$, CLR (1 → 3.7V)

+3.7V → P, T

IC32 E → $\overline{K0}$; B → $\overline{K1}$; C → $\overline{K2}$

K0, K1, K2, K3

AMPLITUDE FREQUENCY AND OFFSET MULTIPLEXING

2A0, 1A0, 0A0 → IC30A LS353 (1C0–1C3, 2C0–2C3, 1Y, 2Y, 1G 2G; K0, K1)

2A1, 1A1, 0A1 → IC30A

2A2, 1A2, 0A2 → IC30B LS353

2A3, 1A3, 0A3 → IC30B

$\overline{K2}$, SDO, $\overline{SD1}$ → IC65 LS10

2F0, 1F0, 0F0 → IC22A LS353

2F1, 1F1, 0F1 → IC22A

IC22B LS353

20F0, 10F0, 00F0 → IC11A LS353

20F1, 10F1, 00F1 → IC11A

20F2, 10F2, 00F2 → IC11B, LS353

20F3, 10F3, 00F3 → IC11B

$\overline{K2}$, SDO, SD2 → IC65

+5V pull-ups: R125 2.21K, R121 2.21K, R119 221K, R126 2.21K, R122 2.21K, R120 2.21K

DISPLAY ENABLE

ITSME → IC39 7474 (K3, N.C., +3.7V)

2-STAR DECODER

IC5 C, IC5 D, IC5 B 7403, IC5 A

R123 2.21K, R124 2.21K

TO DISPLAY BD. (DWG. 0103-00-0105)

IC4 B 7438 → PI-10 DDO

IC4 C 7438 → PI-15 DD1

IC4 D 7438 → PI-11 DD2

IC4 A 7438 → PI-14 DD3

IC3 C 7438 → PI-13 $\overline{D\ SYNC}$

IC3 D → PI-8 $\overline{D\ CLK}$ (B8)

PI-7 DIG COM

+5V → PI-4

N/C → PI-3, PI-5, PI-6, PI-9, PI-12, PI-1, PI-2

-20dB, -40dB → IC38 LS258 (1B, 2B, 3B, 4B; 1A, 2A, 3A, 4A; 1Y, 2Y, 3Y, 4Y; $\overline{AB}$, $\overline{OC}$)

FR0, FR1, FR2

SDO → IC32 F (7404)

$\overline{K2}$, $\overline{K1}$, $\overline{K0}$ → IC28 A (7410)

IC29 A (7400)

(4B2) M AMPL, $\overline{SD1}$, SDO → IC28 C (7410)

MOFFSET, SD1, SDO → IC28 B

OdB → IC31 C (7402)

IC27A LS353 (1C0–1C3, 2C0–2C3, 1Y, 2Y, 1G 2G)

SDO, SD1, F0, F1

$\overline{ENABLE}$

M0, M1, ITSME

M0, M1 → IC31 B (7402)

IC27B LS353

MINUS SIGN FOR AMPLITUDE OR OFFSET AND NO MINUS FOR OdB (x10) AND FREQUENCY FUNCTION AND MODE AND UNIT SELECT MULTIPLEXING.

$\overline{K0}$, $\overline{K1}$, $\overline{K2}$

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN D. COOPER	DATE 1-29-80	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: SCHEMATIC A2 DIGITAL BOARD (DISPLAY LOGIC)
FINISH WAVETEK PROCESS	RELEASE APPROV		
	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1 XX ±.030		
	DO NOT SCALE DWG		MODEL NO 158 159
	SCALE		DWG NO 0103-00-0819 REV B
			CODE IDENT 23338 SHEET 3 OF 6

BISHOP GRAPHICS/ACCUPRESS REORDER NO. A-3894

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

MATCHED SET

R73 30.1K
R74 30.1K
R75 30.1K
R76 30.1K
R78 30.1K
R77 30.1K
R79 301K
R80 301K
R81 301K
R82 301K
R83 301K
R84 301K
R86 10K
R85 6.98K
R87 1M
R89 4.64K
R88 10K
R90 1M
R92 10K
R91 6.98K
R93 1M
R95 11K
R94 4.02K
R96 1M
R97 9.53K
R79 10K
R70 2.49K
R98 21.5K
+15V
R100 4.02
R103 10K
C6 .1UF
R102 10K
R104 3.83K
R105 4.99K
C5 1.1UF 20V
R106 3.83K
R101 56.2K
-15V
IC62 UA741
IC63 UA741

CR58 CR60 CR61 CR63 CR65 CR67 CR69 CR70 CR72 CR74 CR76 CR78 CR80 CR82 CR83

CR57 2A3 (B5)
CR59 2A2 (B5)
CR62 2A1 (B5)
CR64 2A0 (B5)
CR66 1A3 (B4)
CR68 1A2 (B4)
CR71 1A1 (B4)
CR73 1A0 (B4)
CR75 0A3 (B3)
CR77 0A2 (B3)
CR79 0A1 (B3)
CR81 0A0 (B3)

MATCHED SET
MATCHED SET

R107 500Ω
R108 1K
(B1) D/V COM
R109 301K
Q8 2N5461
Q7 NF510
CR84
CR85
D/V (B1)
R111 500Ω
R112 1K
R110 301K
R113 4.99K
+15V
Q9 2N5139
R114 10K
R117 27.4K
-15V
+5V
R116 2.21K
R115 1K
Q6 2N3646

TO ANALOG BD DWG 0103-00-0107 SHZ
P3
(A4) 1 0dB
(A4) 2 -20dB
(A4) 3 -40dB
(C1) 7 } D/V
(C1) 8 }
(C2) 9 } D/V COM
(C2) 10 }

MOST SIGNIFICANT DIGIT
IC26 74175
(B4) 1A1 → 2A1 (C7, 3D5)
(B4) 1A2 → 2A2 (C7, 3D5)
(B4) 1A0 → 2A0 (C6, 3D5)
(B4) 1A3 → 2A3 (C8, 3D5)
IC25 74175
(B3) 0A1 → 1A1 (C5, B5, 3D5)
(B3) 0A2 → 1A2 (C6, B5, 3D5)
(B3) 0A0 → 1A0 (C5, B5, 3D5)
(B3) 0A3 → 1A3 (C6, B5 3D5)
LEAST SIGNIFICANT DIGIT
IC24 74175
D1* (2B7) → 0A1 (C4, B4, 3D5)
D2* (2B7) → 0A2 (C4, B4, 3D5)
D0* (2C7) → 0A0 (C3, B4, 3D5)
D3* (2B7) → 0A3 (C4, B4, 3D5)

AMPL (ASCII) A
I (2D7)
RESA (2B7)
SELA (3C7)
40EC (2C4)
IC19A 7474
SELA (B3)
IC20 C
IC20 B
IC20 A
7410
3.7V
RNGCLK (2C1)
IC19B 7474
30C
SELAR (B3)
40EC
ADRSET

RESA (2B7) 7474
I (2D7)
N.C. IC21A
-20DB (B1, 3C4)
IC31 7402
0DB (3B4, B1)
Z (2D7)
N.C. IC21B
-40DB (B1, 3C4)

SELA (B6)
SELAR (A6)
7408
IC7 A
IC7 B
MSIGN (2D4)
MCLK
IC17B 74107
M AMPL (3C4)
IC3 A
IC3 B
7438
F1 (2C1)
IC1 A
IC1 B
7404
IC6 B
7400

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN C.J. Cox	DATE 3/5/74	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL —	PRODUCTION	4/11/74	TITLE SCHEMATIC A2 DIGITAL BOARD (AMPLITUDE D/A)
FINISH WAVETEK PROCESS —	RELEASE APPROV		
	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° XX ±.030		
	DO NOT SCALE DWG		MODEL NO. 158/159 DWG NO. 0103-00-0819 REV B
	SCALE		CODE IDENT 23338 SHEET 4 OF 6

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

MATCHED SET

R1 30.1K, R2 30.1K, R3 30.1K, R4 30.1K, R6 30.1K, R5 30.1K

CR2, CR4, CR5, CR7, CR9

CR1 — 20F3

CR3 — 20F2 (B5)

CR6 — 20F1 (B5)

CR8 — 20F0 (B5)

MATCHED SET

R7 301K, R8 301K, R9 301K, R10 301K, R12 301K, R11 301K

CR11, CR13, CR14, CR16, CR18

CR10 — 10F3 (B4)

CR12 — 10F2 (B4)

CR15 — 10F1 (B4)

CR17 — 10F0 (B4)

MATCHED SET

R14 10K, R13 6.98K, R15 1M, R17 4.64K, R16 10K, R18 1M, R20 10K, R19 6.98K, R21 1M, R23 11K, R22 4.02K, R24 1M, R26 9.53K, R28 5K, R27 38.3K, R68 2.49K

CR20, CR22, CR24, CR26, CR27

CR19 — 00F3 (B4)

CR21 — 00F2 (B4)

CR23 — 00F1 (B4)

CR25 — 00F0 (B4)

R25 56.2K — -15V

+15V

R29 6.19K

IC59 µA741

R30 1K

-15V

R31 4.99K

IC60 µA741

R33 4.99K

C2 .1µF 20V

R34 1K

R32 4.99K

C1 .1µF 20V

Q1 2N5461

Q2 2N5485

R36 301K

R35 301K

CR28, CR29

R37 4.99K

+15V

Q3 2N5139

R38 10K

R118 27.4K

-15V

+5V

R39 2.21K

R40 2K

Q4 2N3646

M OFFSET (B6)

P3 — DC OFFSET

TO ANALOG BD DWG 0103-00-0107 SH 2

OFST (ASCII) D

4 (2D7), (D OFFSET), 4DEC (2C4)

IC12A 7474

RESB (2B7)

SELOFF (3C7)

+3.7V

30C (2C4)

IC6

ADRSET (2D2)

IC6

IC7 C 7408

MSIGN (2D4)

MCLK (2D6)

IC 17

M OFFSET (B3,3B4)

IC1 C 7404

IC6 C 7400

IC10 74175

(B4) 10F3 — 20F3 (C8,3B5) NC

(B4) 10F2 — 20F2 (C7,3B5) NC

(B4) 10F0 — 20F0 (C7,3B5) NC

(B4) 10F1 — 20F1 (C7,3B5) NC

IC9 74175

00F3 (B4) — 10F3 (B5,C6,3B5) NC

00F1 (B4) — 10F1 (B5,C6,3B5) NC

00F0 (B4) — 10F0 (B5,C6,3B5) NC

00F2 (B4) — 10F2 (B5,C6,3B5) NC

IC8 74175

D3* (2B7) — 00F3 (C4,B5,3B5) NC

D1* (2B7) — 00F1 (C9,B5,3B5) NC

D0*12 (2B7) — 00F0 (C3,B5,3B5) NC

D2* (2B7) — 00F2 (C9,B5,3B5) NC

NOTE. UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE 3/4/74	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL —	PROJ ENGR	6/4/74	TITLE: SCHEMATIC A2 DIGITAL BOARD (OFFSET D/A)
	RELEASE APPROV		
FINISH WAVETEK PROCESS —	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ±.010 ANGLES ±1 XX ±.030		
	DO NOT SCALE DWG		MODEL NO 153/159 — DWG NO 0103-00-0819 — REV B
	SCALE —		CODE IDENT 23338 — SHEET 5 OF 6

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

MATCHED SET

MATCHED SET

MATCHED SET

MATCHED SET

R41 30.1K
R42 30.1K
R43 30.1K
R44 30.1K
R45 30.1K
R46 30.1K
R47 301K
R48 301K
R49 301K
R50 301K
R51 301K
R52 301K
R53 6.98K
R54 10K
R55 1M
R56 10K
R57 4.64K
R58 1M
R59 6.98K
R60 10K
R61 1M
R62 4.02K
R63 11K
R64 1M
R69 2.49K
R71 9.53K
R72 56.2K
R65 46.4Ω
R66 4.99K
R67 3.32K
C4 .1uF 20V
C3 .1UF 20V

+5V
+15V
-15V

CR30 CR31 CR32 CR33 CR34 CR35 CR36 CR37 CR38 CR39 CR40 CR41 CR42 CR43 CR44 CR45 CR46 CR47 CR48 CR49 CR50 CR51 CR52 CR53 CR54 CR55 CR56

2F3 (B6)
2F2 (B6)
2F1 (B6)
2F0 (B6)
1F3 (B4)
1F2 (B4)
1F1 (B4)
1F0 (B4)
0F3 (B3)
0F2 (B3)
0F1 (B3)
0F0 (B3)

IC61 µA741
Q5 2N3638A

TO ANALOG BD DWG 0103-00-0107
P3 39 40 FREQ ADJUST

46 D/F

MOST SIGNIFICANT DIGIT
IC16 74175

(B4) 1F3
(B4) 1F2
(B4) 1F0
(B4) 1F1

2F3(C8,3C5)
2F2(C7, 3C5)
2F0(C7, 3C5)
2F1(C7, 3C5)

IC15 74175

(B3) 0F1
(B3) 0F3
(B3) 0F0
(B3) 0F2

1F1(C5, C6, 3C5)
1F3(B6, C6, 3C5)
1F0(B6, C5, 3C5)
1F2(B6, C6, 3C5)

LEAST SIGNIFICANT DIGIT
IC14 74175

D1* (2B7)
D3* (2B7)
D0* (2B7)
D3* (2B7)

0F1(B5, C4, 3C5)
0F3(B5, C5, 3C5)
0F0(B5, C3, 3C5)
0F2(B5, C4, C35)

IC23 74175

D1* (2B7)
D2* (2B7)
D0* (2C7)
N.C.

FR1 (3C4)
FR2 (3C4)
FR0 (3C4)

35 36 FR1
33 34 FR2
37 38 FR0

IC18A 7474
IC18B 7474

FREQ (ASCII F) (2D7)
40EC (2C4)
RESA (2B7)
SELF (3C7)
RNGCLR
40EC

IC13 D 7410
IC13 B 7410
IC13 A 7410

30C
ADRSET (2D2)

3.7V

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN C.L.Cox	DATE 3/5/74	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL —	PROJ ENGR R.Peterson	6/24/74	TITLE SCHEMATIC A2 DIGITAL BOARD (FREQUENCY D/A)
	RELEASE APPROV		
FINISH WAVETEK PROCESS —	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030		
	DO NOT SCALE DWG		MODEL NO. 158/159 DWG NO. 0103-00-0819 REV B
	SCALE —		CODE IDENT 23338 SHEET 6 OF 6

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

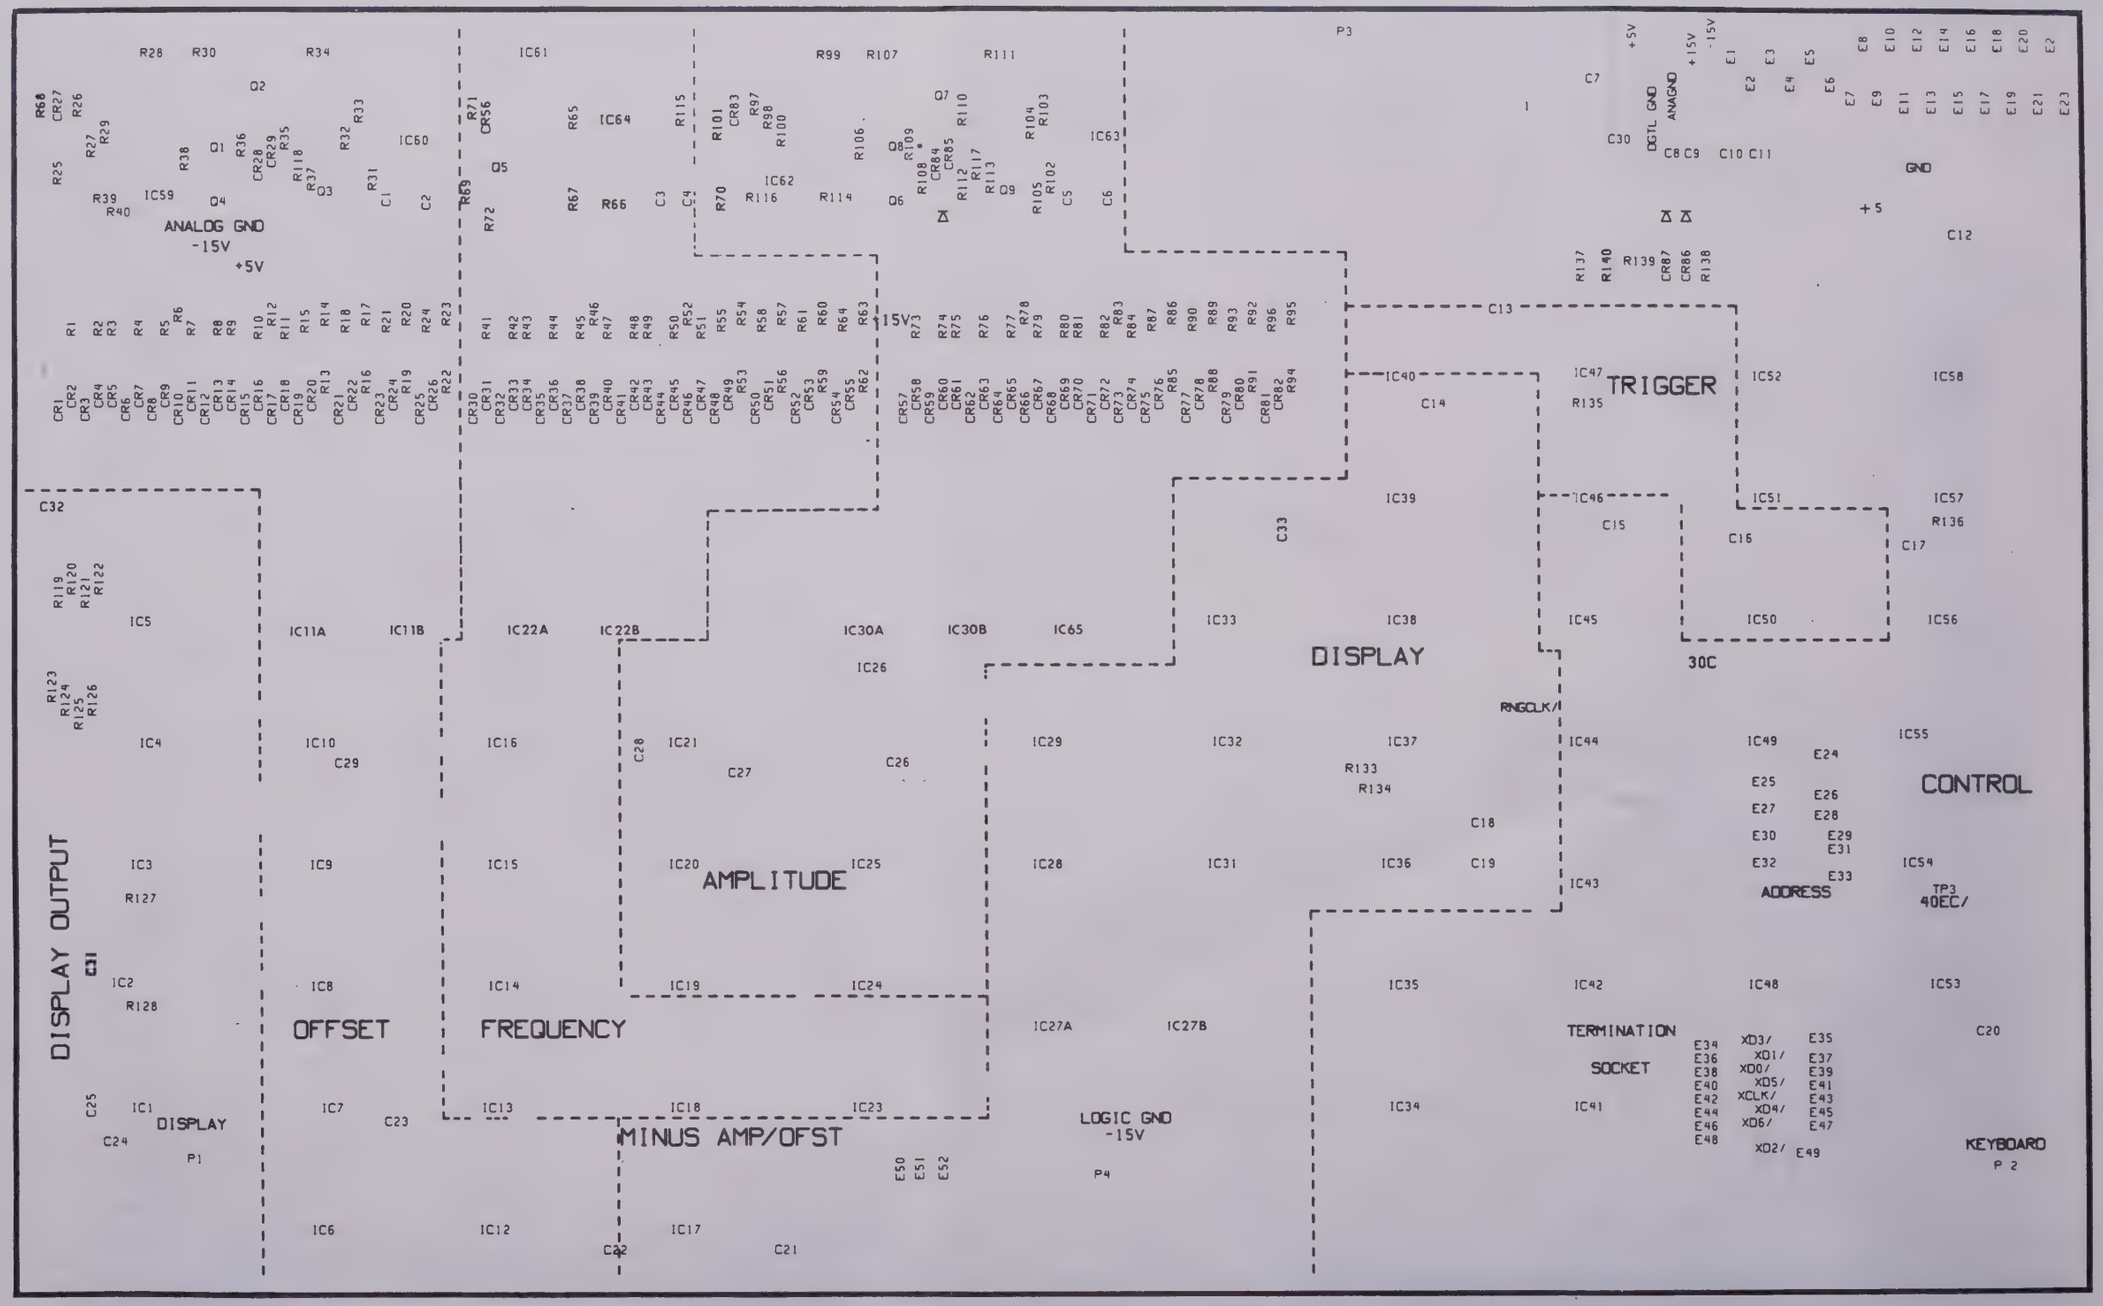

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: PCA DIGITAL BD.
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ± .010 ANGLES ± 1 XX ± .030		
	DO NOT SCALE DWG		MODEL NO 159 · DWG NO 0101-00-0819 · REV
	SCALE		CODE IDENT 23338 · SHEET OF

REV	ECN	BY	DATE	APP

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	ASSY DRWG, DIGITAL BD	0101-00-0819	WVTK	0101-00-0819	1
NONE	SCHEMATIC, DIGITAL BD	0103-00-0819	WVTK	0103-00-0819	1
P3	CABLE ASSY	158-400	WVTK	1207-00-0003	1
NONE	BAR, SUPPORT	158-312	WVTK	1400-00-0683	2
C11 C13 C18 C20 C21 C22 C23 C24 C32 C33 C7 C9	CAP, CER, MN, .01MF, 50V	CAC02Z5U103Z100A	CORNG	1500-01-0310	12
C1 C2 C3 C4 C5 C6	CAP, CER, MON, .1MF, 50V	CAC03Z5U104Z050A	CORNG	1500-01-0405	6
C17	CAP, CER, 33PF, 1KV	DD-330	CRL	1500-03-3011	1
C19 C300	CAP, CER, 470PF, 1KV	DD-471	CRL	1500-04-7111	2
C12	CAP, ELECT, 250MF, 16V	500D257G016DF7	SPRAG	1500-32-5101	1
C10 C27 C28 C8	CAP, TANT, 22MF, 15V	196D226X9015KA1	SPRAG	1500-72-2601	4
C14 C15 C16 C25 C26 C29 C30 C31	CAP, TANT, 33MF, 10V	150D336X9010B2	SPRAG	1500-73-3601	8
NONE	DIGITAL BOARD	1700-00-0819	WVTK	1700-00-0819	1
P1 P2 P5	CONN, 15PIN	03-09-1151	MOLEX	2100-02-0012	3
NONE	PLUG, 15PIN	03-09-2151	MOLEX	2100-02-0013	1
NONE	SKT, IC, 14PIN	CB814-01.	TI	2100-03-0011	1
P4	CONN, EDGE CARD	252-18-30-160	CINCH	2100-03-0013	1

WAVETEK PARTS LIST | TITLE: PCA, DIGITAL BOARD | ASSEMBLY NO. 1100-00-0819 | PAGE: 1 | REV B

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
R116 R119 R120 R121 R122 R123 R124 R125 R126 R128 R135 R39	RES, MF, 1/8W, 1%, 2.21K	RN55D-2211F	TRW	4701-03-2211	12
R68 R69 R70	RES, MF, 1/8W, 1%, 2.49K	RN55D-2491F	TRW	4701-03-2491	3
R138T	RES, MF, 1/8W, 1%, 24.9K	RN55D-2492F	TRW	4701-03-2492	1
R117 R118	RES, MF, 1/8W, 1%, 27.4K	RN55D-2742F	TRW	4701-03-2742	2
R109 R110 R134 R35 R36	RES, MF, 1/8W, 1%, 301K	RN55D-3013F	TRW	4701-03-3013	5
R140 R67	RES, MF, 1/8W, 1%, 3.32K	RN55D-3321F	TRW	4701-03-3321	2
R104 R106	RES, MF, 1/8W, 1%, 3.83K	RN55D-3831F	TRW	4701-03-3831	2
R27	RES, MF, 1/8W, 1%, 38.3K	RN55D-3832F	TRW	4701-03-3832	1
R100 R22 R62 R94	RES, MF, 1/8W, 1%, 4.02K	RN55D-4021F	TRW	4701-03-4021	4
R17 R57 R89	RES, MF, 1/8W, 1%, 4.64K	RN55D-4641F	TRW	4701-03-4641	3
R65	RES, MF, 1.8W, 1%, 46.4	RN55D-46R4F	TRW	4701-03-4649	1
R105 R113 R31 R32 R33 R37 R66	RES, MF, 1/8W, 1%, 4.99K	RN55D-4991F	TRW	4701-03-4991	7
R133	RES, MF, 1/8W, 1%, 49.9K	RN55D-4992F	TRW	4701-03-4992	1
R101 R25 R72	RES, MF, 1/8W, 1%, 56.2K	RN55D-5622F	TRW	4701-03-5622	3
R29	RES, MF, 1/8W, 1%, 6.19K	RN55D-6191F	TRW	4701-03-6191	1

WAVETEK PARTS LIST | TITLE: PCA, DIGITAL BOARD | ASSEMBLY NO. 1100-00-0819 | PAGE: 3 | REV B

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
CR85 CR86 CR87					
CR1 CR10 CR11 CR13 CR14 CR16 CR18 CR2 CR30 CR31 CR33 CR34 CR36 CR38 CR39 CR4 CR40 CR42 CR43 CR45 CR47 CR5 CR57 CR58 CR60 CR61 CR63 CR65 CR66 CR67 CR69 CR7 CR70 CR72 CR74 CR9	DIODE, SET, 6-FD-6666 QTY: 6: 4807-02-6666	154-500-69	WVTK	4898-00-0001	6
Q5	TRANS	2N3638A	CARTR	4901-03-6381	1
Q4 Q6	TRANS	2N3646	NSC	4901-03-6460	2
Q3 Q9	TRANS	2N5139	FAIR	4901-05-1390	2
Q1 Q8	TRANS	2N5461	INTSL	4901-05-4610	2
Q2	TRANS	2N5485	MOT	4901-05-4850	1
Q7	TRANS	MF-510	NSC	4902-00-5100	1
IC36	IC	NE555V	SIG	7000-05-5500	1
IC59 IC60 IC61 IC62 IC63 IC64	IC	LM741CN	NSC	7000-07-4100	6
IC 29 IC49 IC6	IC	7400	TI	8000-74-0000	3
IC31 IC44 IC48	IC	7402	TI	8000-74-0200	3
IC5	IC	7403	TI	8000-74-0300	1

WAVETEK PARTS LIST | TITLE: PCA, DIGITAL BOARD | ASSEMBLY NO. 1100-00-0819 | PAGE: 5 | REV B

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	PIN, FEMALE	02-09-1133	MOLEX	2100-05-0004	30
NONE	PIN, MALE	02-09-2118	MOLEX	2100-05-0005	7
NONE	PIN, MALE	61182-2	AMP	2100-05-0020	6
NONE	PIN, FEMALE	02-09-1118	MOLEX	2100-05-0026	14
NONE	TRANSIPAD	10123N	METRS	2800-11-0003	1
R30 R34	POT, TRIM, 1K	91AR1K	BECK	4600-01-0209	2
R99	POT, TRIM, 10K	91AR10K	BECK	4600-01-0315	1
R107 R111	POT, TRIM, 500	91AR500	BECK	4600-05-0104	2
R28	POT, TRIM, 5K	91AR5K	BECK	4600-05-0205	1
R139	RES, C, 1W, 10%, 1K	RC32GF-102	STKPL	4700-35-1001	1
R137	RES, MF, 1/8W, 1%, 100	RN55D-1000F	TRW	4701-03-1000	1
R108 R112 R115	RES, MF, 1/8W, 1%, 1K	RN55D-1001F	TRW	4701-03-1001	3
R102 R103 R114 R136 R14 R16 R20 R38 R54 R56 R60 R86 R88 R92	RES, MF, 1/8W, 1%, 10K	RN55D-1002F	TRW	4701-03-1002	14
R23 R63 R95	RES, MF, 1/8W, 1%, 11K	RN55D-1102F	TRW	4701-03-1102	3
R40	RES, MF, 1/8W, 1%, 2K	RN55D-2001F	TRW	4701-03-2001	1
R127 R98	RES, MF, 1/8W, 1%, 21.5K	RN55D-2152F	TRW	4701-03-2152	2

WAVETEK PARTS LIST | TITLE: PCA, DIGITAL BOARD | ASSEMBLY NO. 1100-00-0819 | PAGE: 2 | REV B

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
R13 R19 R53 R59 R85 R91	RES, MF, 1/8W, 1%, 6.98K	RN55D-6981F	TRW	4701-03-6981	6
R26 R71 R97	RES, MF, 1/8W, 1%, 9.53K	RN55D-9531F	TRW	4701-03-9531	3
R15 R18 R21 R24 R55 R58 R61 R64 R87 R90 R93 R96	RES, MF, 1/4W, 1%, 1M	RN60D-1004F	TRW	4701-13-1004	12
IC41	RES MODULE	899-5-R220/330	BECK	4770-00-0004	1
R1 R2 R3 R4 R41 R42 R43 R44 R45 R46 R5 R6 R73 R74 R75 R76 R77 R78	RES, SET, 6-30.1K, 1/8W QTY: 6: 4701-03-3012	158-501-94A	WVTK	4789-00-0025	3
R10 R11 R12 R47 R48 R49 R50 R51 R52 R7 R79 R8 R80 R81 R82 R83 R84 R9	RES, SET, 6-301K, 1/8W QTY: 6: 4701-03-3013	157-501-26A	WVTK	4789-00-0030	3
CR12 CR15 CR17 CR19 CR20 CR21 CR22 CR23 CR24 CR25 CR26 CR27 CR28 CR29 CR3 CR32 CR35 CR37 CR41 CR44 CR46 CR48 CR49 CR50 CR51 CR52 CR53 CR54 CR55 CR56 CR59 CR6 CR62 CR64 CR68 CR71 CR73 CR75 CR76 CR77 CR78 CR79 CR8 CR80 CR81 CR82 CR83 CR84	DIODE	1N4148	FAIR	4807-02-6666	51

WAVETEK PARTS LIST | TITLE: PCA, DIGITAL BOARD | ASSEMBLY NO. 1100-00-0819 | PAGE: 4 | REV B

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
IC1 IC32 IC45	IC	7404	TI	8000-74-0400	3
IC58 IC7	IC	7408	TI	8000-74-0800	2
IC13 IC20 IC28 IC33	IC	7410	TI	8000-74-1000	4
IC65	IC	74LS10	TI	8000-74-1010	1
IC52 IC53	IC	7437	TI	8000-74-3700	2
IC3 IC4	IC	7438	TI	8000-74-3800	2
IC12 IC18 IC19 IC21 IC39 IC46 IC50 IC51 IC54 IC57	IC	7474	TI	8000-74-7400	10
IC2 IC56	IC	8601/9601	FAIR	8000-86-0100	2
IC17 IC40 IC55	IC	74107	TI	8007-41-0700	3
IC34 IC42 IC47	IC	74132	TI	8007-41-3200	3
IC35	IC	74LS138	TI	8007-41-3810	1
IC43	IC	74154	FAIR	8007-41-5400	1
IC37	IC	74161	TI	8007-41-6100	1
IC10 IC14 IC15 IC16 IC23 IC24 IC25 IC26 IC8 IC9	IC	74175	TI	8007-41-7500	10
IC38	IC	74LS258	TI	8007-42-5810	1

WAVETEK PARTS LIST | TITLE: PCA, DIGITAL BOARD | ASSEMBLY NO. 1100-00-0819 | PAGE: 6 | REV B

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: PARTS LIST PCA, DIGITAL BOARD
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° XX ±.030		MODEL NO 159 / DWG NO 1100-00-0819 / REV B
	DO NOT SCALE DWG		CODE IDENT 23338 / SHEET 1 OF 2
	SCALE		

BISHOP GRAPHICS/ACCUPRESS RECORDER NO. A-3884

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
IC11A IC11B IC22A IC22B IC27A IC27B IC30A IC30B	IC	74LS353	FAIR	8007-43-5310	8

WAVETEK PARTS LIST	TITLE PCA, DIGITAL BOARD	ASSEMBLY NO. 1100-00-0819 PAGE: 7	REV B

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: PARTS LIST PCA, DIGITAL BD
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1 XX ±.030		MODEL NO 159 / DWG NO 1100-00-0819 / REV B
	DO NOT SCALE DWG		CODE IDENT 23338 / SHEET 2 OF 2
	SCALE		

BISHOP GRAPHICS/ACCUPRESS REORDER NO. A-3894

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	ECN 1308	RL	6-1-77	
B	ECN 1519	RO	2-17-77	
C	3115	fne	5/7/82	
	3194 (CL III)	fne	9/24/82	
D	3768	fne	5/9/83	

UCG AMPLIFIER

GENERATOR ENABLE CIRCUIT

FREQUENCY RANGE LOGIC

COMPARATOR | HYSTERESIS

INTEGRATOR

SQUAREWAVE AMPLIFIER

RAMP AMPLIFIER

SINE CONVERTER & AMPLIFIER

FROM DIGITAL BD DWG 153-218 SHT 6

6. ** NOMINAL VALUE CALLED OUT ON PARTS LIST
5. ALL RESISTOR VALUES IN Ω, 1%, 1/8 W.
4. ALL CAPACITOR VALUES IN μF.
3. ⏚ TO PIN 7 & +5V TO PIN 14 ON IC 4, 5, 6, 15, 16 & 18
2. * = MATCHED SET
1. ALL DIODES ARE FD666666.

NOTE: UNLESS OTHERWISE SPECIFIED

LAST REF DES USED	
CAP	C81
RES	R257
DIODE	CR42
I.C.	IC 18
RELAY	K10
TRANSISTOR	Q43

E	# 3902 # 3956	SC	9-19-83	
F	3794 (CL II)	fne	6-1-83	

REMOVE ALL BURRS AND BREAK SHARP EDGES | MATERIAL | FINISH WAVETEK PROCESS

DRAWN C.L. Cox 4/9/74 | PROJ ENGR | RELEASE/APPROV 6/30/75

TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ±.010 ANGLES ±1° XX ±.030

DO NOT SCALE DWG | SCALE

WAVETEK SAN DIEGO, CALIFORNIA

TITLE: SCHEMATIC ANALOG BOARD A3

MODEL NO. 158/159 | DWG NO. 0103-00-0107 | REV E

CODE IDENT 23338 | SHEET 1 OF 2

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

J3 — DIGITAL COM, ANALOG COM, D/V COM, D/V (TO BG), DC OFFSET

INVERTING AMPLIFIER

OUTPUT AMPLIFIER CIRCUIT

FUNCTION SELECT LOGIC

X-Y MULTIPLIER CIRCUIT

IC17 FOUR QUADRANT MULTIPLIER MC1495L

ATTENUATOR SELECT LOGIC

SINE WAVE FROM 183

TRIANGLE WAVE FROM IC1

D/V (FROM CB)

SQUARE WAVE FROM 1A6

RAMP WAVE FROM 1A5

FROM DIGITAL BD DWG SHEET 2

3 - 40dB

4 ENABLE

2 - 20dB

1 0dB

FROM DIGITAL BD DWG 158-218 SHEET 4

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN C.L. Cox	DATE 4/9/84	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL —	PROCESS APPROV	DATE	TITLE SCHEMATIC ANALOG BOARD A3
FINISH WAVETEK PROCESS —	RELEASE APPROV		
	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030		
	DO NOT SCALE DWG	MODEL NO. 158/159	DWG NO. 0103-00-0107 REV E
	SCALE —	CODE IDENT 23338	SHEET 2 OF 2

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

J	2644	LOU	5-5-81	RBG
K	3115	fm	9/7/82	
	3187 (CL III)	fm	5/20/83	
L	3769	fm	5/4/83	
M	3902	SC	9-19-83	

REV	ECN	BY	DATE	APP
C	ECN 1178	RB	1-7-5	
D	ECN 1303	RO	8-11-78	
E	ECN 1308	RO	6-8-78	
F	ECN 1519	RO	2-1-79	
G	ECN 1754	RO	6-19-79	
H	ECN 2153	LTE	5-14-84	



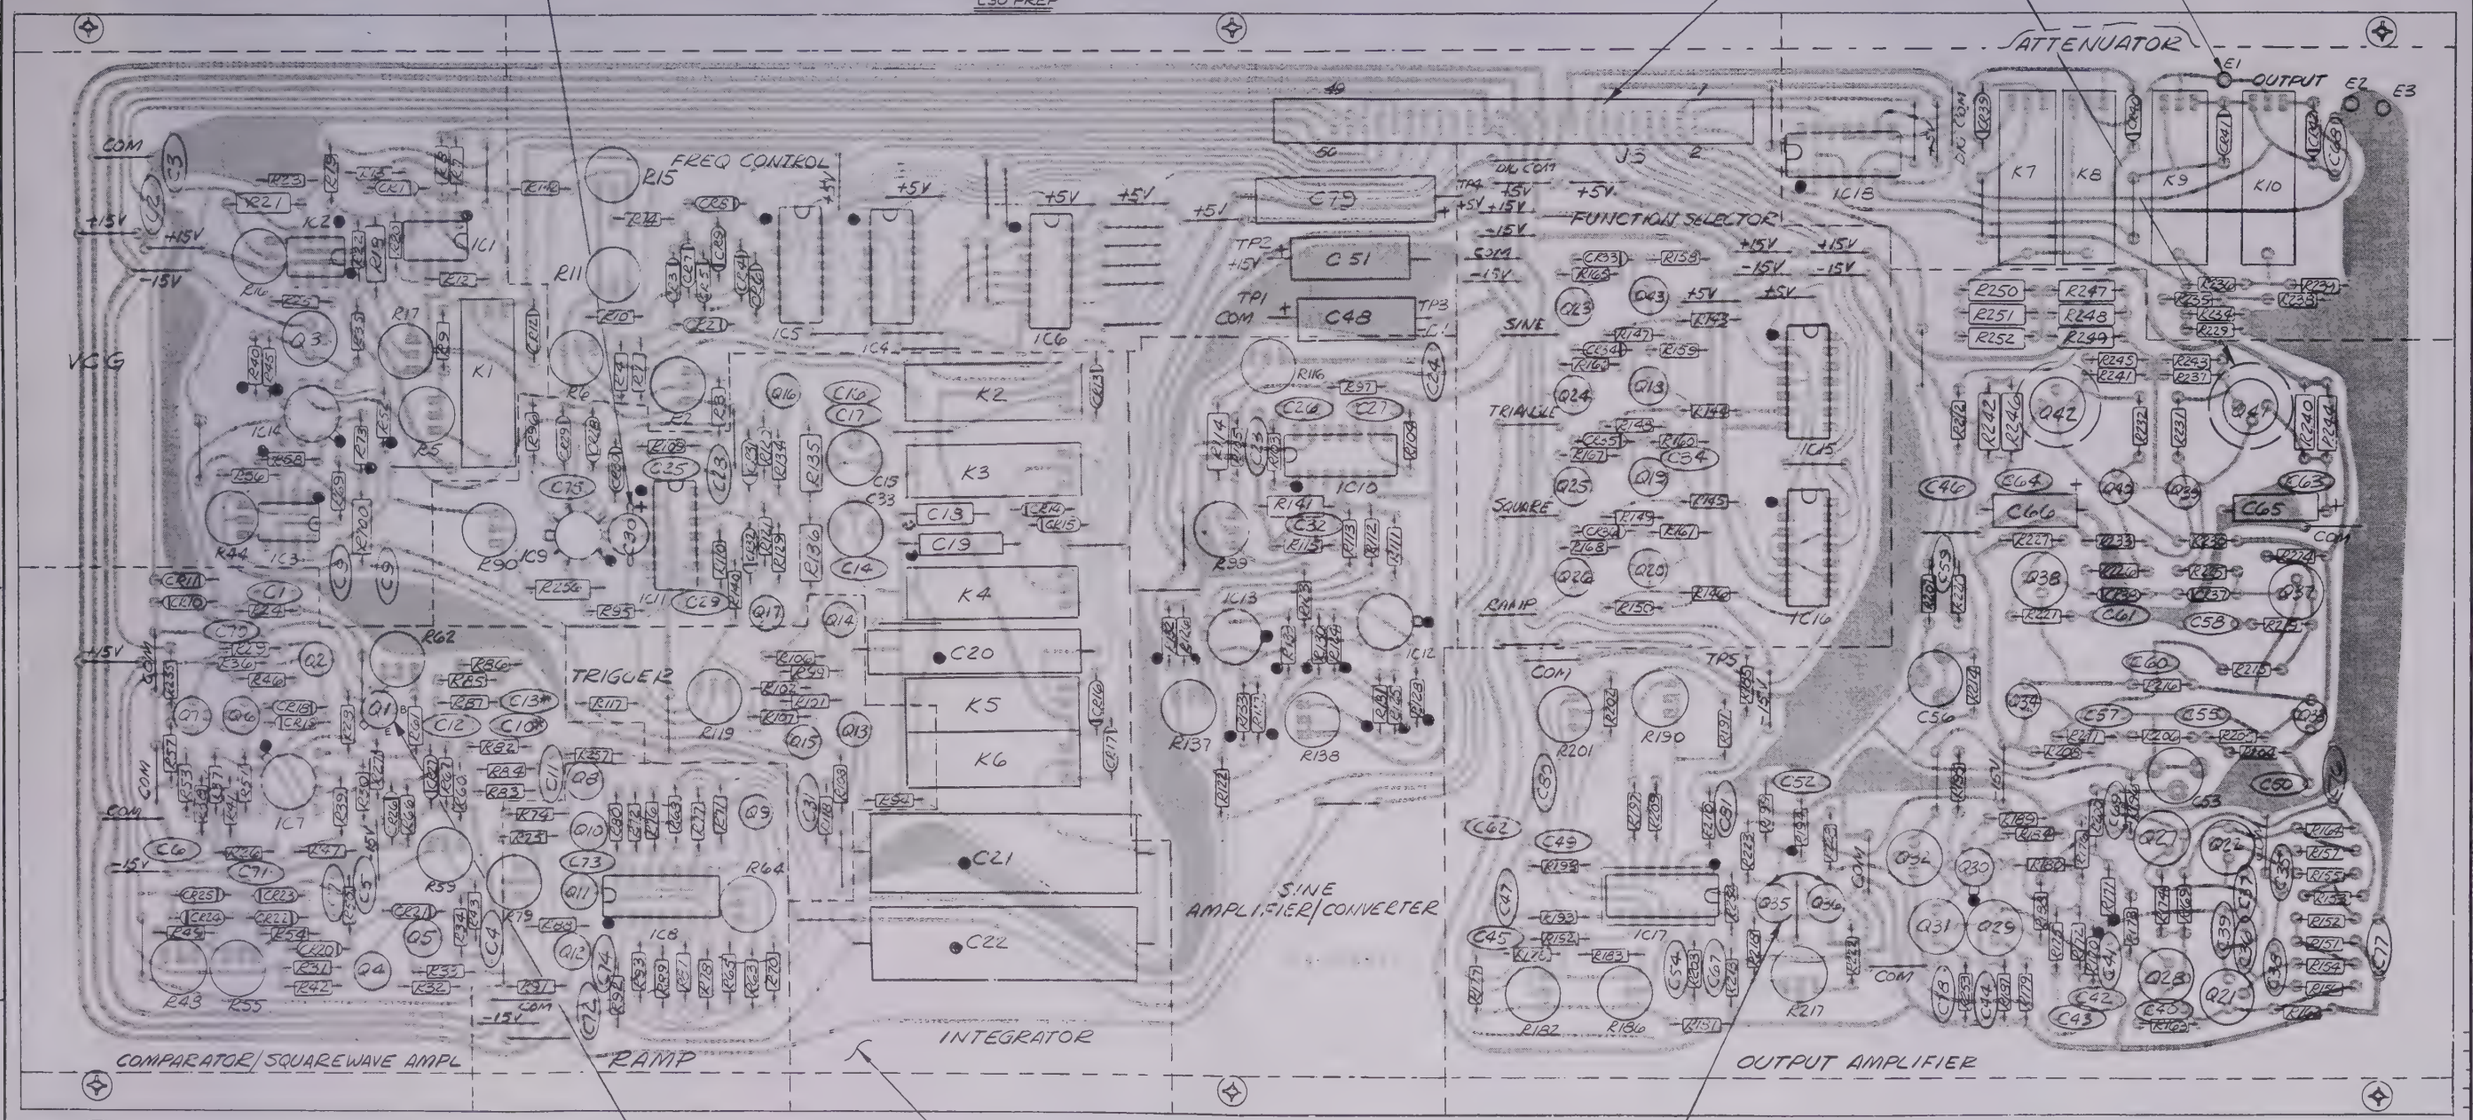

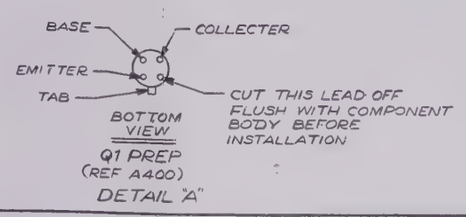

1. *NOMINAL VALUE CALLED OUT ON PARTS LIST

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN C.L. Cox	DATE 4/1/74	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL —	PROJENGR T.P. Williams	1/4/74	TITLE P.C. BOARD ASSEMBLY ANALOG BD
FINISH WAVETEK PROCESS —	RELEASE APPROV R.B.	4/2/5	
	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030		
	DO NOT SCALE DWG	MODEL NO. 158/159	DWG NO. 0101-00-0107 REV M
	SCALE 2:1	CODE IDENT 23338	SHEET 1 OF 1

0101-00-0107

BRUNING 40 520 15821

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	ASSY DRWG, ANALOG	0101-00-0107	WVTK	0101-00-0107	1
NONE	SCHEMATIC, ANALOG	0103-00-0107	WVTK	0103-00-0107	1
176	BAR, SUPPORT	158-312	WVTK	1400-00-0683	2
177	SHIELD	158-319	WVTK	1400-00-0703	1
C39 C59	CAP, CER, 5PF, 1KV	DD-050	CRL	1500-00-5011	2
C1	CAP, CER, 10PF, 1KV	DD-100	CRL	1500-01-0011	1
C31 C43	CAP, CER, 100PF, 1KV	DD-101	CRL	1500-01-0111	2
C34 C35 C36 C37 C38 C4 C42 C44 C45 C47 C5 C54 C55 C57 C6 C60 C63 C64 C67 C81	CAP, CER, MN, .01MF, 50V	CAC02Z5U103Z100A	CORNG	1500-01-0310	20
C2 C23 C24 C25 C3 C46 C49 C50 C58 C61 C62 C68 C70 C71 C72 C76 C77 C78 C8 C80 C9	CAP, CER, MON, .1MF, 50V	CAC03Z5U104Z050A	CORNG	1500-01-0405	21
C32	CAP, CER, 150PF, 1KV	DD-151	CRL	1500-01-5111	1
C26 C27 C28 C29 C41	CAP, CER, 22PF, 1KV	DD-220	CRL	1500-02-2011	5
C74	CAP, CER, 220PF, 1KV	DD-221	CRL	1500-02-2111	1
C52 C7	CAP, CER, 30PF, 1KV	DD-300	CRL	1500-03-0001	2
C40	CAP, CER, 330PF, 1KV	DD-331	CRL	1500-03-3111	1
C75	CAP, CER, 47PF, 1KV	DD-470	CRL	1500-04-7011	1

WAVETEK PARTS LIST | TITLE ANALOG | ASSEMBLY NO. 1100-00-0107 PAGE: 1 | REV M

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
	CAP SET, POLYC MIXED MATCHED SET			1509-80-0005	
C19	CAP, POLYC, .1MF, 100V PART OF 1509-80-0005 QTY(1)				
C20	CAP, POLYC, 1MF, 100V PART OF 1509-80-0005 QTY(1)				
C21 C22	CAP, POLYC, 5MF, 100V PART OF 1509-80-0005 QTY(2)				
172	ANALOG	158-119	WVTK	1700-00-0107	1
170	CONN, HEADER 50 PIN	3433-4005	3M	2100-02-0029	1
NONE	SKT, IC, 14PIN	C8B14-01.	TI	2100-03-0011	1
190	PIN, MALE	61182-2	AMP	2100-05-0020	3
191	HEAT SINK	207	WAKE	2800-11-0001	2
193	TRANSIPAD	10123N	METRS	2800-11-0003	2
192	TRANSIPAD	10160	METRS	2800-11-0004	2
K1 K10 K2 K3 K4 K5 K6 K7 K8 K9	RELAY, REED, FORM-A	RA3019-1051	ETROL	4500-00-0007	10
R217	POT, TRIM, 100	91AR100	BECK	4600-01-0103	1
R48 R55	POT, TRIM, 1K	91AR1K	BECK	4600-01-0209	2

WAVETEK PARTS LIST | TITLE ANALOG | ASSEMBLY NO. 1100-00-0107 PAGE: 3 | REV M

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
R88					
R82 R87	RES, MF, 1/8W, 1%, 12.1K	RN55D-1212F	TRW	4701-03-1212	2
R113	RES, MF, 1/8W, 1%, 124	RN55D-1240F	TRW	4701-03-1240	1
R106 R207 R63	RES, MF, 1/8W, 1%, 13K	RN55D-1302F	TRW	4701-03-1302	3
R175	RES, MF, 1/8W, 1%, 130K	RN55D-1303F	TRW	4701-03-1303	1
R123	RES, MF, 1/8W, 1%, 150	RN55D-1500F	TRW	4701-03-1500	1
R31 R34 R72 R9 R93	RES, MF, 1/8W, 1%, 1.5K	RN55D-1501F	TRW	4701-03-1501	5
R158 R159 R160 R161	RES, MF, 1/8W, 1%, 15K	RN55D-1502F	TRW	4701-03-1502	4
R156 R157 R219 R221 R237 R241 R243 R245	RES, MF, 1/8W, 1%, 15	RN55D-15R0F	TRW	4701-03-1509	8
R7	RES, MF, 1/8W, 1%, 15.8K	RN55D-1582F	TRW	4701-03-1582	1
R179 R212 R253 R71	RES, MF, 1/8W, 1%, 1.78K	RN55D-1781F	TRW	4701-03-1781	4
R8	RES, MF, 1/8W, 1%, 178K	RN55D-1783F	TRW	4701-03-1783	1
R112 R224	RES, MF, 1/8W, 1%, 200	RN55D-2000F	TRW	4701-03-2000	2
R120 R121 R140 R202 R209 R218 R222 R29 R30 R46 R53 R97 R99	RES, MF, 1/8W, 1%, 2K	RN55D-2001F	TRW	4701-03-2001	13
R184 R189	RES, MF, 1/8W, 1%, 21.5	RN55D-21R5F	TRW	4701-03-2159	2
R200	RES, MF, 1/8W, 1%, 221	RN55D-2210F	TRW	4701-03-2210	1

WAVETEK PARTS LIST | TITLE ANALOG | ASSEMBLY NO. 1100-00-0107 PAGE: 5 | REV M

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
C69	CAP, CER, 470PF, 1KV	DD-471	CRL	1500-04-7111	1
C73	CAP, CER, 82PF, 1KV	DD-820	CRL	1500-08-2011	1
C11 C12	CAP, MICA, 120PF, 500V	DM15-121J	ARCO	1500-11-2100	2
C10T C13T	CAP, MICA, 30PF, 500V	DM15-300J	ARCO	1500-13-0000	2
C16	CAP, MICA, 56PF, 500V	DM15-560J	ARCO	1500-15-6000	1
C14	CAP, MICA, 68PF, 500V	DM15-680F	ARCO	1500-16-8001	1
C17	CAP, MICA, 820PF, 300V	DM15-821F	ARCO	1500-18-2101	1
C48 C51	CAP, ELECT, 100MF, 16V	300D107G016DC7	SPRAG	1500-31-0101	2
C30	CAP, ELECT, 100MF/16V RADIAL LEAD, SP .20	CRE SERIES 100/16	CAPAR	1500-31-0111	1
C79	CAP, ELECT, 250MF, 16V	300D257G016DF7	SPRAG	1500-32-5101	1
C15 C33 C53 C56	VARI, 7-35PF, 250V	7S-TRIKD-02 7/35 PF	TRIKO	1500-53-5000	4
C65 C66	CAP, TANT, 5.6MF, 35V	150D565X9035B2	SPRAG	1500-75-6502	2
	CAP SET, POLYC MIXED MATCHED SET	130-301-6	WVTK	1509-80-0005	1
C18	CAP, POLYC, .01MF, 100V PART OF 1509-80-0005 QTY(1)				

WAVETEK PARTS LIST | TITLE ANALOG | ASSEMBLY NO. 1100-00-0107 PAGE: 2 | REV M

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
R182 R186 R44	POT, TRIM, 10K	91AR10K	BECK	4600-01-0315	3
R11 R116 R119 R15 R16 R17 R190 R2 R201 R6 R90	POT, TRIM, 100K	91AR100K	BECK	4600-01-0402	11
R137 R138	POT, TRIM, 200	91AR200	BECK	4600-02-0101	2
R79	POT, TRIM, 2K	91AR2K	BECK	4600-02-0201	1
R5 R59 R62 R64 R98	POT, TRIM, 500	91AR500	BECK	4600-05-0104	5
R240 R242 R244 R246	RES, C, 1/2W, 5%, 27	RC20GF-270	STKPL	4700-25-0270	4
R135 R136	RES, C, 1/2W, 5%, 4.7	RC20GF-4R7	STKPL	4700-25-0479	2
R254 R39 R41 R77 R80 R83 R86 R92	RES, MF, 1/8W, 1%, 100	RN55D-1000F	TRW	4701-03-1000	8
R115 R177 R178 R255 R36 R57 R95	RES, MF, 1/8W, 1%, 1K	RN55D-1001F	TRW	4701-03-1001	7
R107 R108 R118 R169 R181 R183 R223 R228 R35 R38	RES, MF, 1/8W, 1%, 10K	RN55D-1002F	TRW	4701-03-1002	10
R117	RES, MF, 1/8W, 1%, 100K	RN55D-1003F	TRW	4701-03-1003	1
R185 R32 R33 R76 R81	RES, MF, 1/8W, 1%, 10	RN55D-10R0F	TRW	4701-03-1009	5
R188 R91	RES, MF, 1/8W, 1%, 11K	RN55D-1102F	TRW	4701-03-1102	2
R103 R104 R215 R75	RES, MF, 1/8W, 1%, 1.21K	RN55D-1211F	TRW	4701-03-1211	5

WAVETEK PARTS LIST | TITLE ANALOG | ASSEMBLY NO. 1100-00-0107 PAGE: 4 | REV M

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
R143 R144 R145 R146 R180 R195	RES, MF, 1/8W, 1%, 2.21K	RN55D-2211F	TRW	4701-03-2211	6
R187 R213	RES, MF, 1/8W, 1%, 2.37K	RN55D-2371F	TRW	4701-03-2371	2
R152	RES, MF, 1/8W, 1%, 23.7K	RN55D-2372F	TRW	4701-03-2372	1
R172	RES, MF, 1/8W, 1%, 237K	RN55D-2373F	TRW	4701-03-2373	1
R109 R110 R235 R24 R26 R37	RES, MF, 1/8W, 1%, 249	RN55D-2490F	TRW	4701-03-2490	6
R151 R153 R176 R204 R208 R236 R49 R54	RES, MF, 1/8W, 1%, 2.49K	RN55D-2491F	TRW	4701-03-2491	8
R192 R193	RES, MF, 1/8W, 1%, 274	RN55D-2740F	TRW	4701-03-2740	2
R96	RES, MF, 1/8W, 1%, 27.4K	RN55D-2742F	TRW	4701-03-2742	1
R163 R205 R211 R214 R56	RES, MF, 1/8W, 1%, 3.01K	RN55D-3011F	TRW	4701-03-3011	5
R230 R233 R74	RES, MF, 1/8W, 1%, 30.1K	RN55D-3012F	TRW	4701-03-3012	3
R165 R166 R167 R168	RES, MF, 1/8W, 1%, 301K	RN55D-3013F	TRW	4701-03-3013	4
R111 R220 R50 R94	RES, MF, 1/8W, 1%, 316	RN55D-3160F	TRW	4701-03-3160	4
R70	RES, MF, 1/8W, 1%, 332	RN55D-3320F	TRW	4701-03-3320	1
R13 R23	RES, MF, 1/8W, 1%, 3.32K	RN55D-3321F	TRW	4701-03-3321	2
R10 R14 R206 R4	RES, MF, 1/8W, 1%, 33.2K	RN55D-3322F	TRW	4701-03-3322	4

WAVETEK PARTS LIST | TITLE ANALOG | ASSEMBLY NO. 1100-00-0107 PAGE: 6 | REV M

NOTE. UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: PARTS LIST ANALOG
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ±.010 ANGLES ±1° XX ± .030		MODEL NO. 159 / DWG NO. 1100-00-0107 / REV M
	DO NOT SCALE DWG		CODE IDENT 23338 / SHEET 1 OF 2
	SCALE		

BISHOP GRAPHICS/ACCUPRESS REORDER NO. A-3894

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
R257	RES, MF, 1/8W, 1%, 33.2	RN55D-33R2F	TRW	4701-03-3329	1
R1	RES, MF, 1/8W, 1%, 38.3K	RN55D-3832F	TRW	4701-03-3832	1
R162 R164 R227	RES, MF, 1/8W, 1%, 392	RN55D-3920F	TRW	4701-03-3920	3
R173 R78	RES, MF, 1/8W, 1%, 4.32K	RN55D-4321F	TRW	4701-03-4321	2
R84 R85	RES, MF, 1/8W, 1%, 464	RN55D-4640F	TRW	4701-03-4640	2
R129 R134 R25 R69	RES, MF, 1.8W, 1%, 46.4	RN55D-46R4F	TRW	4701-03-4649	4
R191	RES, MF, 1/8W, 1%, 47.5K	RN55D-4752F	TRW	4701-03-4752	1
R231 R232 R66 R67	RES, MF, 1/8, 1%, 499	RN55D-4990F	TRW	4701-03-4990	4
R12 R147 R148 R149 R150 R19 R27 R68 R89	RES, MF, 1/8W, 1%, 4.99K	RN55D-4991F	TRW	4701-03-4991	9
R142	RES, MF, 1/8W, 1%, 49.9K	RN55D-4992F	TRW	4701-03-4992	1
R239	RES, MF, 1/8W, 1%, 51.1	RN55D-51R1F	TRW	4701-03-5119	1
R198	RES, MF, 1/8W, 1%, 56.2	RN55D-56R2F	TRW	4701-03-5629	1
R174 R60 R61	RES, MF, 1/8W, 1%, 5.76K	RN55D-5761F	TRW	4701-03-5761	3
R102 R154 R155 R216	RES, MF, 1/8W, 1%, 6.19K	RN55D-6191F	TRW	4701-03-6191	4
R225 R226 R238	RES, MF, 1/8W, 1%, 61.9	RN55D-61R9F	TRW	4701-03-6199	3
R101 R20 R3	RES, MF, 1/8W, 1%, 6.81K	RN55D-6811F	TRW	4701-03-6811	3
R199 R234	RES, MF, 1/8W, 1%, 68.1	RN55D-68R1F	TRW	4701-03-6819	2

WAVETEK PARTS LIST | TITLE ANALOG | ASSEMBLY NO. 1100-00-0107 | PAGE: 7 | REV M

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
	RES, MF, MIXED SET	130-501-5A	WVTK	4789-00-0032	1
R124 R125 R126 R127	RES, MF, 1/8W, 1%, 15K PART OF 4789-00-0032 QTY(4)				
R128 R139	RES, MF, 1/8W, 1%, 23.7K PART OF 4789-00-0032 QTY(2)				
R130 R131	RES, MF, 1/8W, 1%, 69.8K PART OF 4789-00-0032 QTY(2)				
R132 R133	RES, MF, 1/8W, 1%, 178K PART OF 4789-00-0032 QTY(2)				
CR22 CR23 CR24 CR25 CR26 CR27	DIODE	FD777	FAIR	4807-02-0777	6
CR1 CR10 CR11 CR12 CR13 CR14 CR15 CR16 CR17 CR18 CR19 CR2 CR20 CR21 CR28 CR29 CR3 CR30 CR31 CR32 CR33 CR34 CR35 CR36 CR37 CR38 CR39 CR4 CR40 CR41 CR42 CR5 CR6 CR7 CR8 CR9	DIODE	1N4148	FAIR	4807-02-6666	36
Q38 Q41	TRANS	2N2219A	NSC	4901-02-2191	2
Q37 Q42	TRANS	2N2905A	NSC	4901-02-9051	2

WAVETEK PARTS LIST | TITLE ANALOG | ASSEMBLY NO. 1100-00-0107 | PAGE: 9 | REV M

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
R203 R210	RES, MF, 1/8W, 1%, 6.98K	RN55D-6981F	TRW	4701-03-6981	2
R28 R47 R51	RES, MF, 1/8W, 1%, 750	RN55D-7500F	TRW	4701-03-7500	3
R229	RES, MF, 1/8W, 1%, 825	RN55D-8250F	TRW	4701-03-8250	1
R105 R197 R42 R43	RES, MF, 1/8W, 1%, 8.25K	RN55D-8251F	TRW	4701-03-8251	4
R122	RES, MF, 1/8W, 1%, 82.5	RN55D-82R5F	TRW	4701-03-8259	1
R65	RES, MF, 1/8W, 1%, 909	RN55D-9090F	TRW	4701-03-9090	1
R114 R18 R21	RES, MF, 1/4W, 1%, 1M	RN60D-1004F	TRW	4701-13-1004	3
R141	RES, MF, 1/4W, 1%, 49.9	RN60D-49R9F	TRW	4701-13-4999	1
R247 R248 R249 R250 R251 R252	RES, MF, 1/4W, 1%, 75	RN60D-75R0F	TRW	4701-13-7509	6
R100 R256	RES, MF, 1/4W, 1%, 825K	RN60D-8253F	TRW	4701-13-8253	2
R171 R196	RES, SET, 2-1.5K, 1/8W QTY: 2: 4701-03-1501	158-501-95A	WVTK	4789-00-0008	1
R170 R194	RES, SET, 2-3.01K, 1/8W QTY: 2: 4701-03-3011	157-501-28A	WVTK	4789-00-0012	1
R22 R40 R45 R52 R58 R73	RES, SET, 6-6.19K, 1/8W QTY: 6 4701-03-6191	130-501-3A	WVTK	4789-00-0016	1

WAVETEK PARTS LIST | TITLE ANALOG | ASSEMBLY NO. 1100-00-0107 | PAGE: 8 | REV M

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
Q14 Q33	TRANS	2N3563	FAIR	4901-03-3630	2
Q21 Q27 Q29 Q3 Q31 Q32	TRANS	2N3638A	CARTR	4901-03-6381	6
Q10 Q11 Q13 Q15 Q2 Q34 Q6	TRANS	2N3640	FAIR	4901-03-6400	7
Q22 Q28	TRANS	2N3642	FAIR	4901-03-6420	2
Q39 Q4 Q7 Q9	TRANS	2N3646	NSC	4901-03-6460	4
Q16	TRANS	2N3903	NSC	4901-03-9030	1
Q17	TRANS	2N3905	ITT	4901-03-9050	1
Q12 Q18 Q19 Q20 Q40 Q43 Q5 Q8	TRANS	2N5139	FAIR	4901-05-1390	8
Q1	TRANS	A-400	AMPRX	4902-00-4000	1
Q23 Q24 Q25 Q26	TRANS	NF-510	NSC	4902-00-5100	4
Q35 Q36	TRANS, M/PR, 2N3563 QTY: 2: 4901-03-3630	142-501-52	WVTK	4998-00-0004	1
IC1 IC2 IC3	IC	LM741CN	NSC	7000-07-4100	3
IC9 Q30	IC	AD 812	ANDEV	7000-08-1200	2
IC17	IC	MC1495L	MOT	7000-14-9500	1
IC12 IC13	IC	CA-3019	FAIR	7000-30-1900	2

WAVETEK PARTS LIST | TITLE ANALOG | ASSEMBLY NO. 1100-00-0107 | PAGE: 10 | REV M

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
IC7	IC	CA3049T	RCA	7000-30-4900	1
IC8	IC	CA-3054	RCA	7000-30-5400	1
IC11	IC, CLASS I, CA-3030 QTY: 1: 7000-30-3000	130-501-15	WVTK	7200-00-0001	1
IC10	IC, CLASS II, CA-3030 QTY: 1: 7000-30-3000	130-501-16	WVTK	7200-00-0002	1
IC14	IC, CLASS I, CA-3039 QTY: 1: 7000-30-3900	130-501-18	WVTK	7200-00-0004	1
IC6	IC	4006	MOT	8000-40-0600	1
IC15 IC16 IC4	IC	7400	TI	8000-74-0000	3
IC18	IC	7403	TI	8000-74-0300	1
IC5	IC	7404	TI	8000-74-0400	1

WAVETEK PARTS LIST | TITLE ANALOG | ASSEMBLY NO. 1100-00-0107 | PAGE: 11 | REV M

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: PARTS LIST ANALOG
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX: .010 ANGLES: 1° XX: .030		
	DO NOT SCALE DWG	MODEL NO. 159	DWG NO 1100-00-0107 REV M
	SCALE	CODE IDENT 23338	SHEET 2 OF 2

BISHOP GRAPHICS/ACCUPRESS REORDER NO. A-3894

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	CHG DWG NO. FROM 159-001 ECN1161		9/27	
B	ECN 1160	RL	12/16/82	
C	KBRD ASSY WAS 158-016 DELETED ITEM 10 154-331 ECN 1131			
D	ECN 1288	RL	6/25/84	
E	ECN 1754	RO	6/21/88	

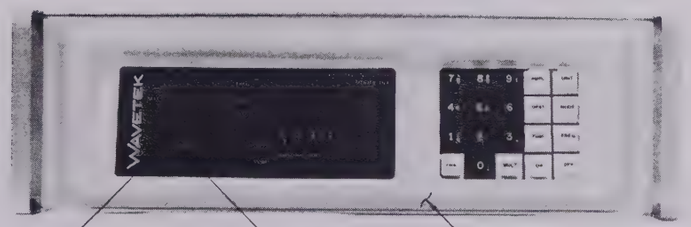

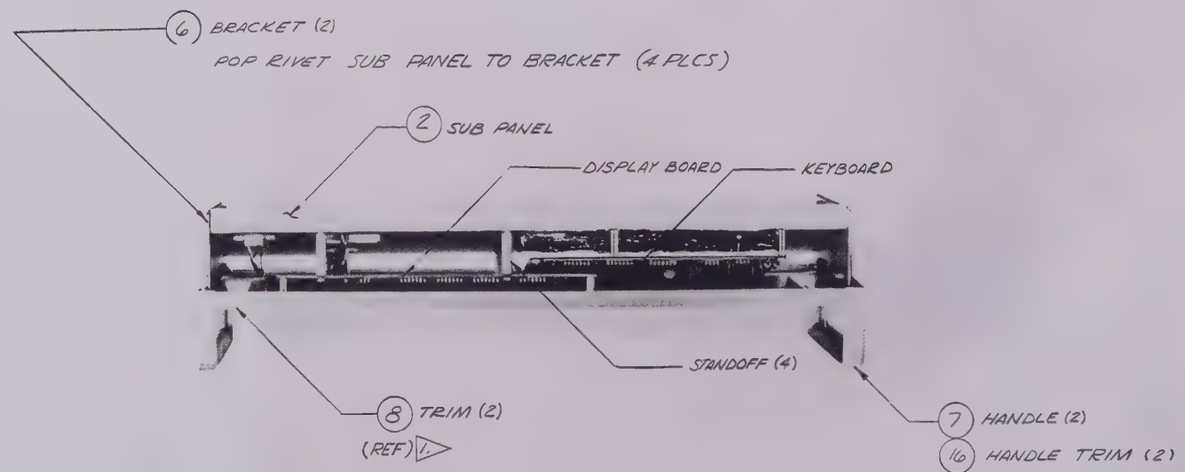

1. INSTALL SHIM SPACER BEHIND FRONT PANEL USING 1/4" DOUBLE SIDED TAPE, BEFORE ADDING TRIM.

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN C.L. Cox 5/24/84	WAVETEK SAN DIEGO, CALIFORNIA	
MATERIAL ——	PROJ ENGR K.P. Schwanke 6/11/84	TITLE ASSEMBLY FRONT PANEL	
	RELEASE APPROV LPS 6/30/85		
FINISH WAVETEK PROCESS ——	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ±.010 ANGLES ±1 XX ±.030		
	DO NOT SCALE DWG	MODEL NO 159	DWG NO. 0102-00-0333 REV E
	SCALE NONE	CODE IDENT 23338	SHEET / OF /

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	ASSY DRWG, FRONT PNL	0102-00-0333	WVTK	0102-00-0333	1
1	PANEL, FT REF: 3200-03-0002	158-309	WVTK	1400-00-0660	1
3	PANEL, FLEX FROM: 1400-00-0691	158-314	WVTK	1400-00-0690	1
2	PANEL, SUB	158-323	WVTK	1400-00-0723	1
6	BRKT	158-324	WVTK	1400-00-0733	2
7	HANDLE, R/A FROM: 1400-00-3561	147-364	WVTK	1400-00-3589	2
16	TRIM, HANDLE REF 3200-06-0006	147-345	WVTK	1400-00-3619	2
14	SHIM, SPACER	1400-00-7003	WVTK	1400-00-7003	2
8	TRIM REF 3200-06-0005	1400-00-7019	WVTK	1400-00-7019	2
NONE	STANDOFF 1.062 H, .250 HEX 6-32	8221-A-0632	AMTOM	2800-02-0012	4

WAVETEK PARTS LIST	TITLE FT PANEL ASSY	ASSEMBLY NO. 1101-00-0075 PAGE: 1	REV E

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE PARTS LIST FT PANEL ASSY
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ±.010 ANGLES ±1° XX ±.030		
	DO NOT SCALE DWG	MODEL NO 159	DWG NO 1101-00-0075 REV E
	SCALE	CODE IDENT 23338	SHEET 1 OF 1

BISHOP GRAPHICS/ACCUPRESS
REORDER NO. A-3884

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	ECN 1754	RD	6-20-77	

KEYBOARD ARRANGEMENT

7	8	9	F	G
4	5	6	A	C
1	2	3	D	B
~	0	E	H	I

A = AMPL
B = MODE
C = FUNC
D = OFST
E = MULT
F = FREQ
G = UNIT
H = ON
I = OFF
~ = CHS

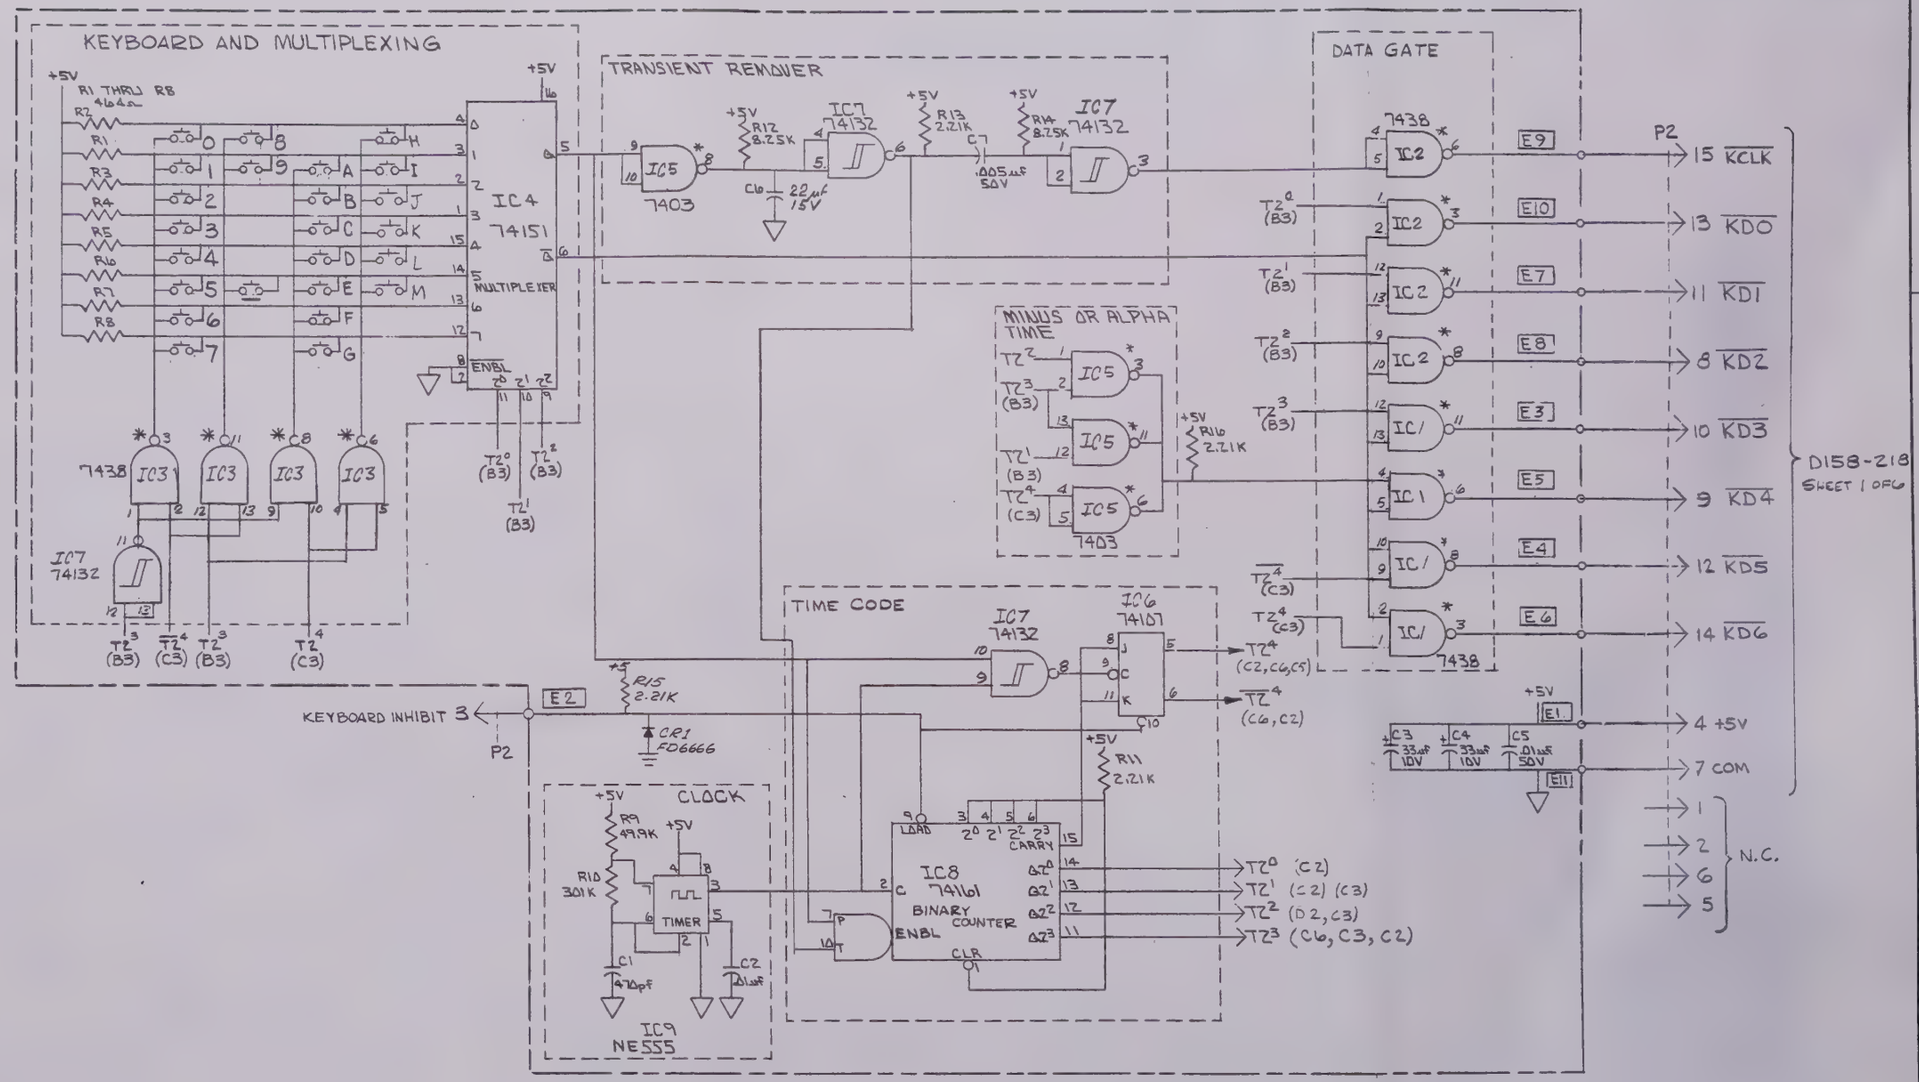

5. ○ DENOTES WIRE COLORS PER RESISTOR COLOR CODES.
4. ▭ DENOTES ACTUAL LABELING.
3. BAR OVER MNEMONIC DENOTES TRUE-WHEN-LOW.
2. * DENOTES OPEN COLLECTOR.
1. ALL RESISTORS ARE ±1% 1/8W.

NOTE: UNLESS OTHERWISE SPECIFIED.

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE 11/19	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR	12/8/75	TITLE: SCHEMATIC KEY BOARD A6
FINISH WAVETEK PROCESS	RELEASE APPROV		
	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030		
	DO NOT SCALE DWG		MODEL NO. 159
	SCALE		DWG NO. 0103-00-0109 REV A
			CODE IDENT 23338 SHEET 1 OF 1

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	ECN 1754	KPO	6-20-78	

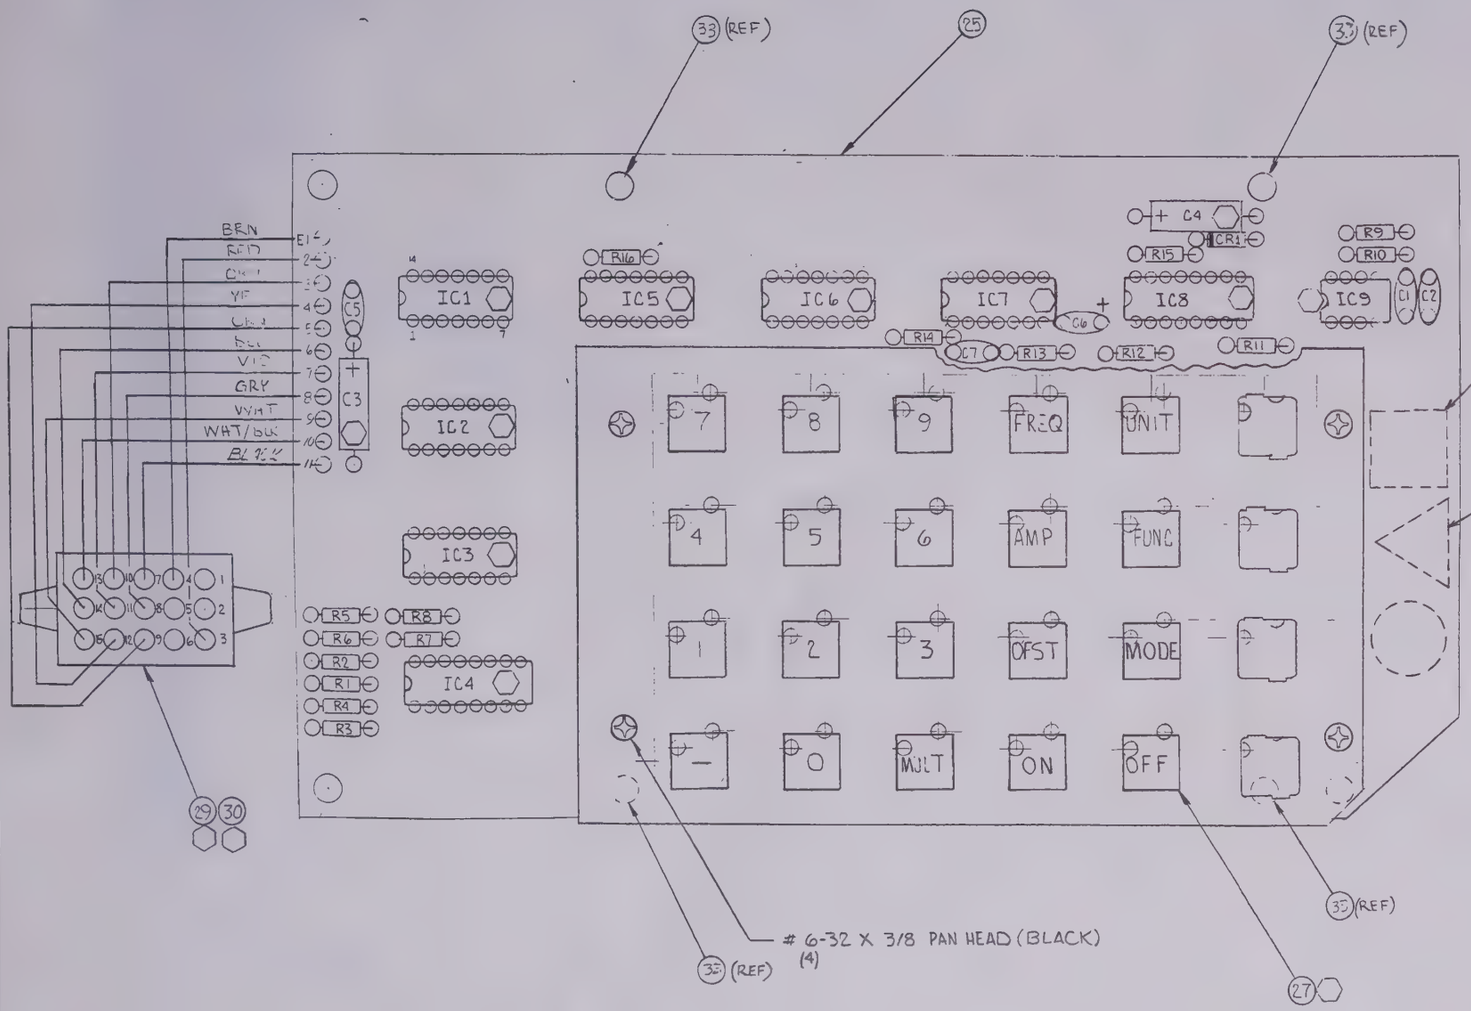

(6)
1. (4) ⬭ NUMBERS IN HEX AND CIRCLES INDICATE STATION LOCATION.

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN D. BARNETT	DATE 12/11/74	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL	ENGINEERING [signature]	1/7/75	TITLE PC ASSY- KEYBOARD
	RELEASE APPROV KB		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ± .010 ANGLES ± 1 XX ± .030		
	DO NOT SCALE DWG	MODEL NO 159	DWG NO 0101-00-0100 REV A
	SCALE 2/1	CODE IDENT 23338	SHEET 1 OF 1

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	DRIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	ASSY DRWG, KEYBOARD	0101-00-0109	WVTK	0101-00-0109	1
NONE	SCHEMATIC, KEYBOARD	0103-00-0109	WVTK	0103-00-0109	1
35	CARRIER, KEY	158-344	WVTK	1400-00-0783	1
C2 C5	CAP, CER, MN, .01MF, 50V	CAC02Z5U103Z100A	CORNG	1500-01-0310	2
C1	CAP, CER, 470PF, 1KV	DD-471	CRL	1500-04-7111	1
C7	CAP, CER, .005MF, 50V	CK-502	CRL	1500-05-0210	1
C6	CAP, TANT, 22MF, 15V	196D226X9015KA1	SPRAG	1500-72-2601	1
C3 C4	CAP, TANT, 33MF, 10V	150D336X9010B2	SPRAG	1500-73-3601	2
25	KEY BOARD	158-147	WVTK	1700-00-0109	1
30	PLUG, 15PIN	03-09-2151	MOLEX	2100-02-0013	1
29	PIN, MALE	02-09-2118	MOLEX	2100-05-0005	11
33	STANDOFF, SMAGE .500 H, .250 HEX 6-32, .062 MAT'L	1331B-1/2-11	USECO	2800-02-0003	4
32	STANDOFF, SMAGE .625 H, .250 HEX 6-32, .062 MAT'L	1331B-5/8	USECO	2800-02-0004	4
R11 R13 R15 R16	RES, MF, 1/8W, 1%, 2.21K	RN55D-2211F	TRW	4701-03-2211	4
R10	RES, MF, 1/8W, 1%, 301K	RN55D-3013F	TRW	4701-03-3013	1
R1 R2 R3 R4 R5 R6 R7	RES, MF, 1/8W, 1%, 464	RN55D-4640F	TRW	4701-03-4640	8

WAVETEK PARTS LIST	TITLE KEY BOARD	ASSEMBLY NO. 1100-00-0109 PAGE: 1	REV A

REFERENCE DESIGNATORS	PART DESCRIPTION	DRIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
R8					
R9	RES, MF, 1/8W, 1%, 49.9K	RN55D-4992F	TRW	4701-03-4992	1
R12 R14	RES, MF, 1/8W, 1%, 8.25K	RN55D-8251F	TRW	4701-03-8251	2
CR1	DIODE	1N4148	FAIR	4807-02-6666	1
27	KEY & SWITCH KIT	159-531	WVTK	5108-00-0001	1
IC9	IC	NE555V	SIG	7000-05-5500	1
IC5	IC	7403	TI	8000-74-0300	1
IC1 IC2 IC3	IC	7438	TI	8000-74-3800	3
IC6	IC	74107	TI	8007-41-0700	1
IC7	IC	74132	TI	8007-41-3200	1
IC4	IC	74151	TI	8007-41-5100	1
IC8	IC	74161	TI	8007-41-6100	1

WAVETEK PARTS LIST	TITLE KEY BOARD	ASSEMBLY NO. 1100-00-0109 PAGE: 2	REV A

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL	PROJ ENGR		TITLE PARTS LIST KEY BOARD
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ±.010 ANGLES ±1 XX ±.030		
	DO NOT SCALE DWG		MODEL NO 159 / DWG NO 1100-00-0109 / REV A
	SCALE		CODE IDENT 23338 / SHEET 1 OF 1

BISHOP GRAPHICS/ACCUPRESS REORDER NO. A-3894

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	REVERSED INPUT/OUTPUT ON A5-3 & 4. CHANGED A2-9 HOOK-UP TO A2-8	MAE	5-5-95	

FROM LOGIC INTERFACE BD

+5V
DIG COM
D SYNC
D CLK
DD3
DD2
DD1
DD0

NO CONNECTION

P1

R146, 58, 59 2.21K

R1 221Ω
R2 332Ω
R3 221Ω
R4 332Ω
R5 221Ω
R6 332Ω
R7 221Ω
R8 332Ω
R9 221Ω
R10 332Ω
R11 221Ω
R12 332Ω

74164 SHIFT REGISTER
SER IN A4
DIG 1 (B1)
DIG 2 (B4)
DIG 3 (B3)
DIG 4 (B3)
DIG 5 (B6)
DIG 6 (B6)
DIG 7 (A6)
DIG 8 (R2, C6)
+3.5V

A3 7400

9370 B1
A (C2)
B (C2)
C (C3)
D (C3)
E (C4)
F (C4)
G (C4)
NC

7474 A2

DIG 8 (D5)
ANGL/ (D5)
DIG 9
DIG 5 (D5)
DIG 6 (D5)
DIG 7 (D5)

C1 74175
D4 74175
D3 74175
D5 4006

(C6) ANGL/
A5 8863
Q9 2N3640
Q8 2N3640
R13 15Ω
R14 332Ω
R15 6.8K
R16 332Ω
R17 6.8K
R18 15Ω
NDP (C4)
ADP (C3)
E10 ⚠
E9

NOT USED ON 159

+5V
C1 33µf 10V
C2—C8 .01µf, 50V

Q7 2N3640
Q6 2N3640
Q5 2N3640
Q4 2N3640
Q3 2N3640
Q2 2N3640
Q1 2N3640
R40 274Ω
R21 15Ω
R24 15Ω
R27 15Ω
R30 15Ω
R33 15Ω
R36 15Ω
R41 274Ω
R39 15Ω

FND357/TIL313 DS8
FND357/TIL313 DS7
FND357/TIL313 DS6
FND357/TIL313 DS5
FND357/TIL313 DS4
FND357/TIL313 DS3
FND357/TIL313 DS2
FND357/TIL313 DS1
NOT USED ON 159
CHANNEL
(MINUS)
MULTIPLER
DIG 2 (D5)
DIG 3 (D5)
DIG 4 (D5)
DIG 8 (D5)
DIG 1 (D5)

SIN
COS
TRI
DC
SQR
ASQR
CONT
TRIG
GATED
SELECTED
NOT USED ON 152

7438
C2
ANGLE
FREQ
OFFSET
AMPL
CR14
CR11
CR13
CR12

TYP FND357 PIN NUMBERS
TYP TIL313 PIN NUMBERS
CATH

4. ○ DENOTES WIRE COLOR PER COLOR CODE.
3. ▭ DENOTES LABELING ON BOARD OR DISPLAY PANEL.
2. ALL RESISTORS ARE ±1%, 1/8W.
⚠ ADD JUMPER WHEN LOADING FOR MODEL 159.

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN MAE	DATE 4-3-95	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROGRAMMER	5/26/95	TITLE: SCHEMATIC— DISPLAY BOARD
FINISH WAVETEK PROCESS	RELEASE APPROV	5/26/95	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ± .010 ANGLES ± 1° XX ± .030
	DO NOT SCALE DWG		MODEL NO 152/159
	SCALE —		DWG NO. 0103-00-0105 REV A
	CODE IDENT 23338		SHEET 1 OF 1

WIRING CHART		
BOARD LOCATION	CODED WIRE COLOR	CONNECTOR PIN NUMBER
E1	1	8
E2	2	10
E3	3	14
E4	4	11
E5	5	15
E6	6	13
E7	0	7
E8	7	4

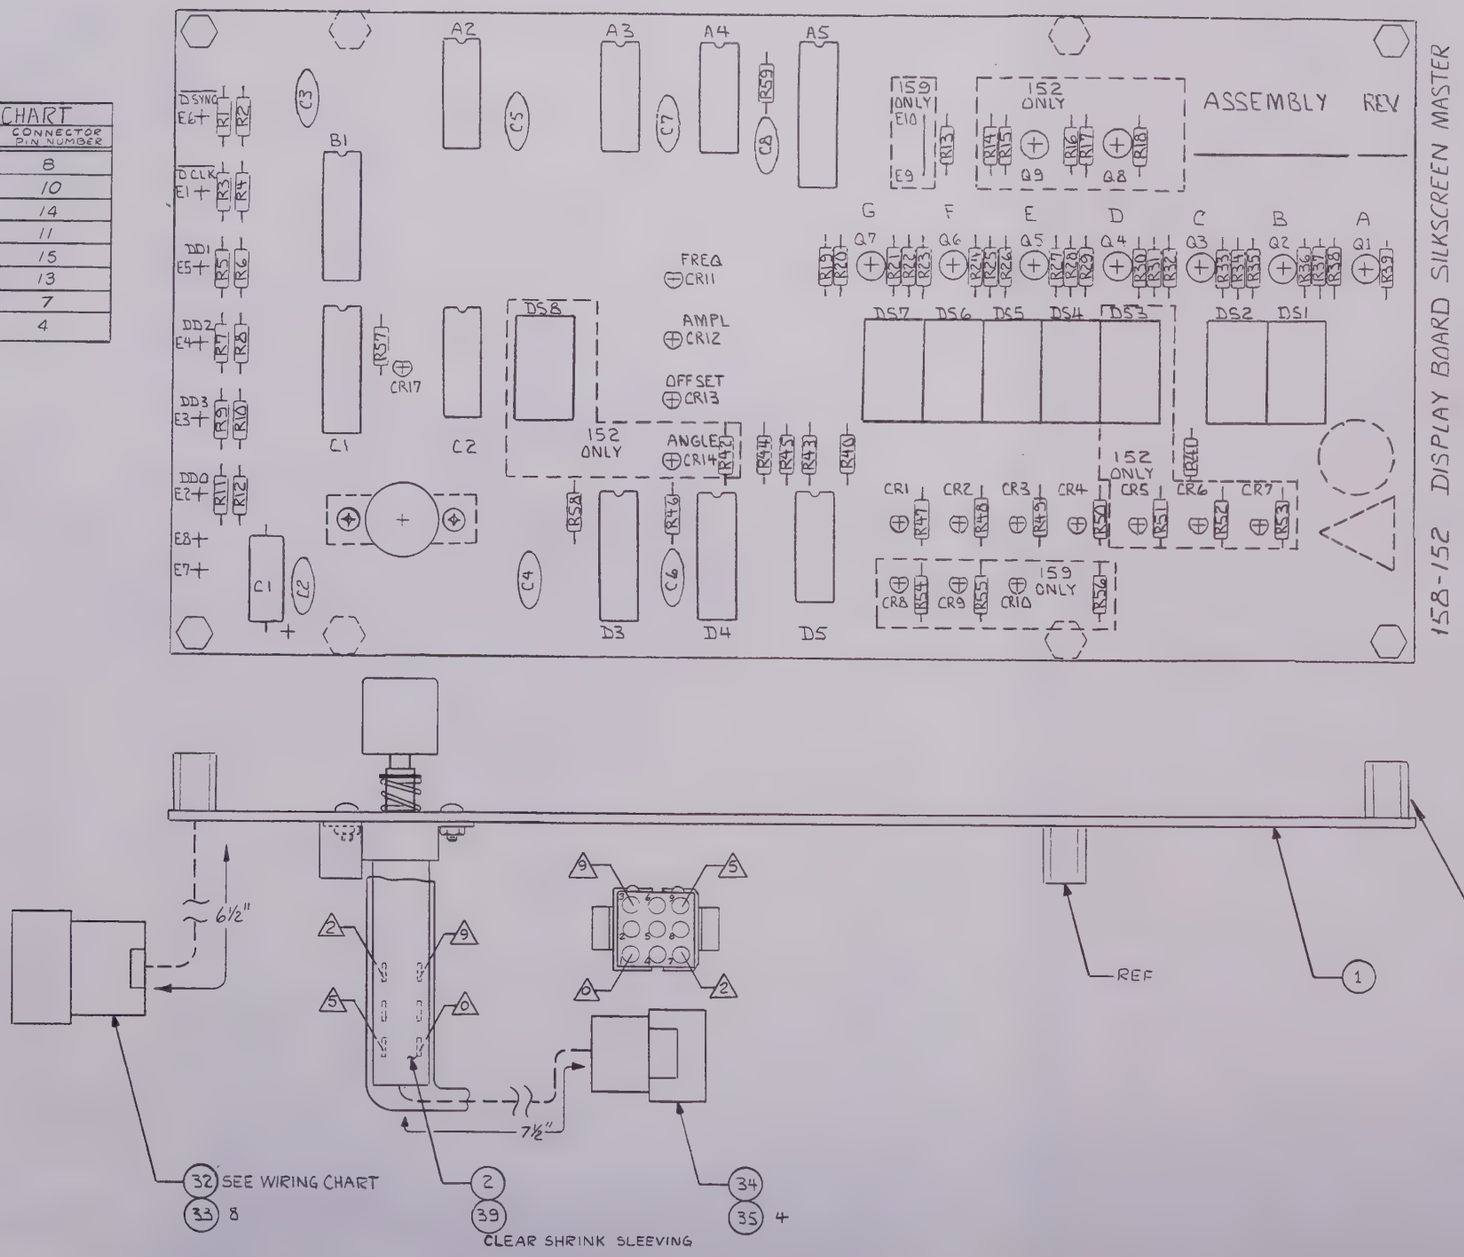

NOTES: 1. △DENOTES WIRE COLOR PER COLOR CODE.

		A	ECN 1314	R0 6-23-75
	DRAWN HAE	DATE 5.9.75	WAVETEK	
MATERIAL SEE PARTS LIST	PROGRAM LP Alverson	5/24/5	TITLE SILKSCREEN ASSEMBLY DWG - DISPLAY BOARD	
	RELEASE ORDER	6/25		
	SCALE 2/1		MODEL NO.	DWG NO. 0101-00-0105 REV A
			CODE IDENT 23338	SHEET 1 OF 1

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	ASSY DRWG, DISPLAY	0101-00-0105	WVTK	0101-00-0105	1
NONE	SCHEMATIC, DISPLAY	0103-00-0105	WVTK	0103-00-0105	1
C2 C3 C4 C5 C6 C7 C8	CAP, CER, MN, .01MF, 50V	CAC02Z5U103Z100A	CORNC	1500-01-0310	7
C1	CAP, TANT, 33MF, 10V	150D336X9010B2	SPRAG	1500-73-3601	1
1	DISPLAY	158-151	WVTK	1700-00-0105	1
34	PLUG, 9PIN	03-06-2091	MOLEX	2100-02-0011	1
32	PLUG, 15PIN	03-09-2151	MOLEX	2100-02-0013	1
35	PIN, MALE	02-06-2103	MOLEX	2100-03-0003	4
33	PIN, MALE	02-09-2118	MOLEX	2100-03-0005	8
38	STANDOFF, SWAGE .375 H, .250 DIA 6-32, .062 MAT'L	6910-6-2C	LYNTR	2800-03-0002	4
R13 R21 R24 R27 R30 R33 R36 R39	RES, MF, 1/8W, 1%, 15	RN55D-15R0F	TRW	4701-03-1509	8
R1 R11 R3 R5 R7 R9	RES, MF, 1/8W, 1%, 221	RN55D-2210F	TRW	4701-03-2210	6
R46 R38 R39	RES, MF, 1/8W, 1%, 2.21K	RN55D-2211F	TRW	4701-03-2211	3
R40 R41 R43 R44 R45 R47 R48 R49 R50 R54 R55 R56 R57	RES, MF, 1/8W, 1%, 274	RN55D-2740F	TRW	4701-03-2740	13
R10 R12 R19 R2 R22	RES, MF, 1/8W, 1%, 332	RN55D-3320F	TRW	4701-03-3320	13

WAVETEK PARTS LIST | TITLE DISPLAY | ASSEMBLY NO. 1100-00-0105 | PAGE: 1 | REV B

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
R25 R28 R31 R34 R37 R4 R6 R8					
R20 R23 R26 R29 R32 R35 R38	RES, MF, 1/8W, 1%, 6.81K	RN55D-6811F	TRW	4701-03-6811	7
CR1 CR10 CR11 CR12 CR13 CR17 CR2 CR3 CR4 CR8 CR9	LED	TIL209A	TI	4899-00-0005	11
DS1 DS2 DS4 DS5 DS6 DS7	LED	HDSP-3106	HP	4899-00-0009	6
Q1 Q2 Q3 Q4 Q5 Q6 Q7	TRANS	2N3640	FAIR	4901-03-6400	7
2	SWITCH ASSY PB	157-422	WVTK	5103-00-0011	1
39	PUSH BUTTON, BLACK	B315 BLACK	CRL	5103-04-0001	1
ICD5	IC	4006	MOT	8000-40-0600	1
ICA3	IC	7400	TI	8000-74-0000	1
ICC2	IC	7438	TI	8000-74-3800	1
ICA2	IC	7474	TI	8000-74-7400	1
ICA5	IC	DS8863	NSC	8000-88-6300	1
ICB1	IC	9370DC	FAIR	8000-93-7000	1
ICA4	IC	74164	TI	8007-41-6400	1
ICC1 ICD3 ICD4	IC	74175	TI	8007-41-7500	3

WAVETEK PARTS LIST | TITLE DISPLAY | ASSEMBLY NO. 1100-00-0105 | PAGE: 2 | REV B

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: PARTS LIST DISPLAY
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1 .XX ±.030		
	DO NOT SCALE DWG	MODEL NO 159	DWG NO 1100-00-0105 REV B
	SCALE	CODE IDENT 23338	SHEET 1 OF 1

BISHOP GRAPHICS/ACCUPRESS REORDER NO. A-3334

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	ECN 1368	RO	11/10/75	
B	ECN 1525	RO	3-1-77	
C	ECN 1754	RO	6-21-78	
D	# 1920		3-7-79	
E	# 2038	DP	10-11-79	
	#3750	DC	5-1-80	

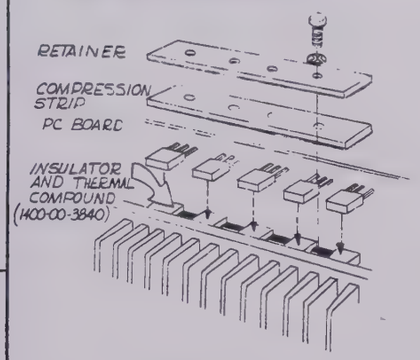

DETAIL "A"

SEE POWER SUPPLY (1100-00-0108) FOR INSTALLATION OF Q1, Q6, Q7 & Q8 (LEADS MUST BE FULL LENGTH)

Q6 Q1 Q8 Q7

E22 E23 E20 E12 E5 E4 E13 E14 E10 E3 E15 E16 E17

(32) (10)
(15) (1)

SW1 (19) SW2 (20)

H1 LD 230 115

FASTEN BOTH SWITCHES WITH 4EA. 4-40 X 1/4 PAN HEAD & #4 MIN. LOCKWASHER & #4 MIN. NUT.

(16) (4) (29)

(1)

4 CONN CABLE

(54) 18GA

(21) (REF)

2EA 4-40 X 1/2 BLACK OXIDE PAN HEAD & #4 MIN. LOCKWASHER & #4 MIN. NUT.

18GA

SAFETY EARTH GROUND LUG

(2)

(REF) (11) (4)
(REF) (12) (4)
(REF) (13) (4)
(14) (4)
(REF)

50Ω OUT
SYNC OUT
TRIG IN
VCG IN
(23)

18GA

(17) (3) AMP FAR END

ADD NYLON SHOULDER WASHERS (TYP 4 PLACES)

(17) (6) AMP FAR END

AT FINAL ASSY THIS CONN IS FROM DIGITAL BD. (158-01B)

(15) (3)

1204-00-0481
WAVETEK

(10) REF

(54)

(8)
(9)

SECURE TRANSFORMER WITH 4 EA 8-32 X 2 1/4 PAN HEAD BLK OXIDE & #8 NUT & LOCKWASHER. (2 EA GO THRU BOARD)

SEE DETAIL "A"

COMPRESSION STRIP

7 EA 6-32 X 1/2 PAN HEAD BLACK OXIDE & 2 EA #6 NUT AND LOCK WASHER

(23)

SECURE TRANSISTORS WITH 4 EA #6-32 X 3/4 PAN HEAD AND #6 LOCK WASHER

(30) (REF) WAKEFIELD COMPOUND (TYP 4 PL)

(23) (4) (REF)

(22) (REF)

2. SLEEVE AS REQUIRED TYP.
1. NUMBERS INDICATE WIRE LOCKS
NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN ADKINS	DATE 6-2-74	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE ASSEMBLY POWER SUPPLY (REAR CASTING)
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ± .010 ANGLES ± 1° .XX ± .030		
	DO NOT SCALE DWG		MODEL NO 158/159 DWG NO 0102-00-0332 REV E
	SCALE		CODE IDENT 23338 SHEET 1 OF 3

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	DDC #1463	DC	9/1678	

SEE SHEET 1

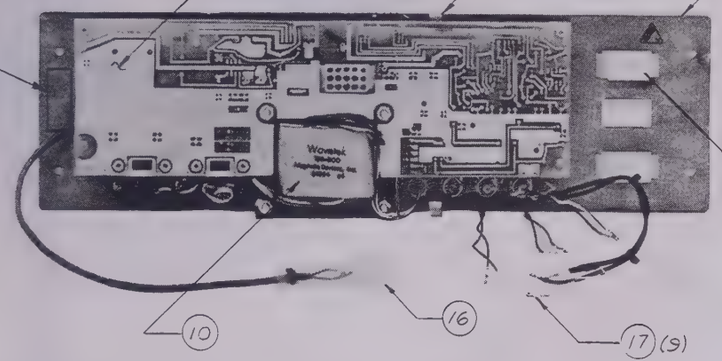

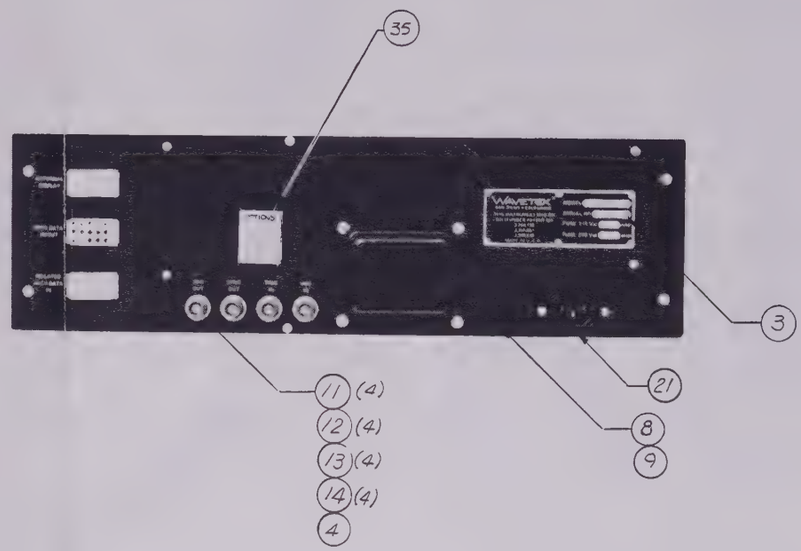

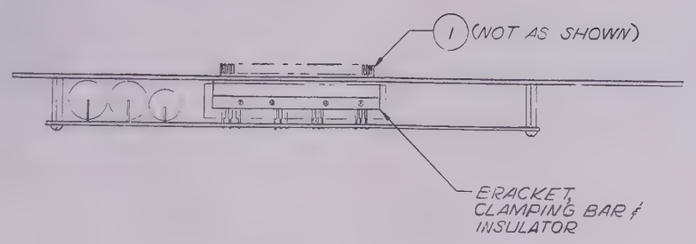

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN C.L. Cox	DATE 5/6/78	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL —	PROJ MGR L.P. Schmidt	6/1/78	TITLE ASSEMBLY REAR PANEL
	RELEASE APPROV		
FINISH WAVETEK PROCESS —	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ± .010 ANGLES ± 1 XX ± .030		
	DO NOT SCALE DWG	MODEL NO 158/159	DWG NO 0102-00-0332 REV E
	SCALE NONE	CODE IDENT 23338	SHEET 2 OF 2

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	ASSY DRWG, REAR PNL	0102-00-0332	WVTK	0102-00-0332	1
10	TRANSFORMER	158-500	WVTK	1204-00-0481	1
2	EXTENDER	158-322	WVTK	1400-00-0710	1
1	CAST, REAR FROM: 1400-00-3671	158-335	WVTK	1400-00-0759	1
30	INSULATOR	147-367	WVTK	1400-00-3700	1
22	BAR, CLAMP	147-379	WVTK	1400-00-3733	1
4	DECAL, BNC	162-309	WVTK	1400-00-3810	1
NONE	STRIP, COMP REF: 3200-08-0001	162-312	WVTK	1400-00-3840	1
NONE	LABEL, OPTION	1400-00-8880	WVTK	1400-00-8880	1
3	I.D. LABEL	1400-00-9110	WVTK	1400-00-9110	1
11	BNC CONN	KC-7946	KING	2100-01-0002	4
16	CONN, 9PIN	03-06-1091	MOLEX	2100-02-0010	1
15	CONN, 15PIN	03-09-1151	MOLEX	2100-02-0012	3
21	RECEPT, POWER	EAC-301	SWCFT	2100-03-0005	1
14	SOLDER LUG	1497	SMITH	2100-04-0012	4
NONE	SOLDER LUG	1485-6	SMITH	2100-04-0025	2
29	PIN, FEMALE	02-06-1103	MOLEX	2100-05-0002	5

WAVETEK PARTS LIST	TITLE REAR PANEL ASSY	ASSEMBLY NO. 1101-00-0074 PAGE: 1	REV G

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
17	CONN	60598-8	AMP	2100-05-0017	9
32	PIN, FEMALE	02-09-1118	MOLEX	2100-05-0026	10
8	FUSE, 3/4A, 250V, S-B	313-750	LITFU	2400-05-0011	1
9	FUSE HOLD	031.1633/031.1666	SCHUR	2400-05-0012	1
23	SPEEDNUT, TYPE"U"	C18050-632-4	TINN	2800-09-0002	6
12	WASHER, SHOULDER	2668	SMITH	2800-27-0004	4
13	NYLON FLAT WASHER	2264-N-385	AMTOM	2800-28-0005	4
19	SW ASSY SLIDE HI-LO	SW422-FT-HK	UID	5105-00-0001	1
20	SWITCH ASSY SLIDE	46256-LF	SWCFT	5105-00-0002	1
31	SOLDER GUARD	46256-LF-SG	SWCFT	5105-09-0001	2

WAVETEK PARTS LIST	TITLE REAR PANEL ASSY	ASSEMBLY NO. 1101-00-0074 PAGE: 2	REV G

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE PARTS LIST REAR PANEL ASSY
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ± .010 ANGLES ± 1 .XX ± .030		
	DO NOT SCALE DWG		MODEL NO 159 / DWG NO 1101-00-0074 / REV G
	SCALE		CODE IDENT 23338 / SHEET 1 OF 1

SHOP GRAPHICS/ACCUPRESS
REORDER NO. A-3894

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	1063	FL	8/20	
B	ECN 1754	RO	1.30.78	
C	# 1920	[illegible]	2-21-79	
D	3072	[illegible]	3/5/79	
—	3795 (CL III)	[illegible]	6/11/79	

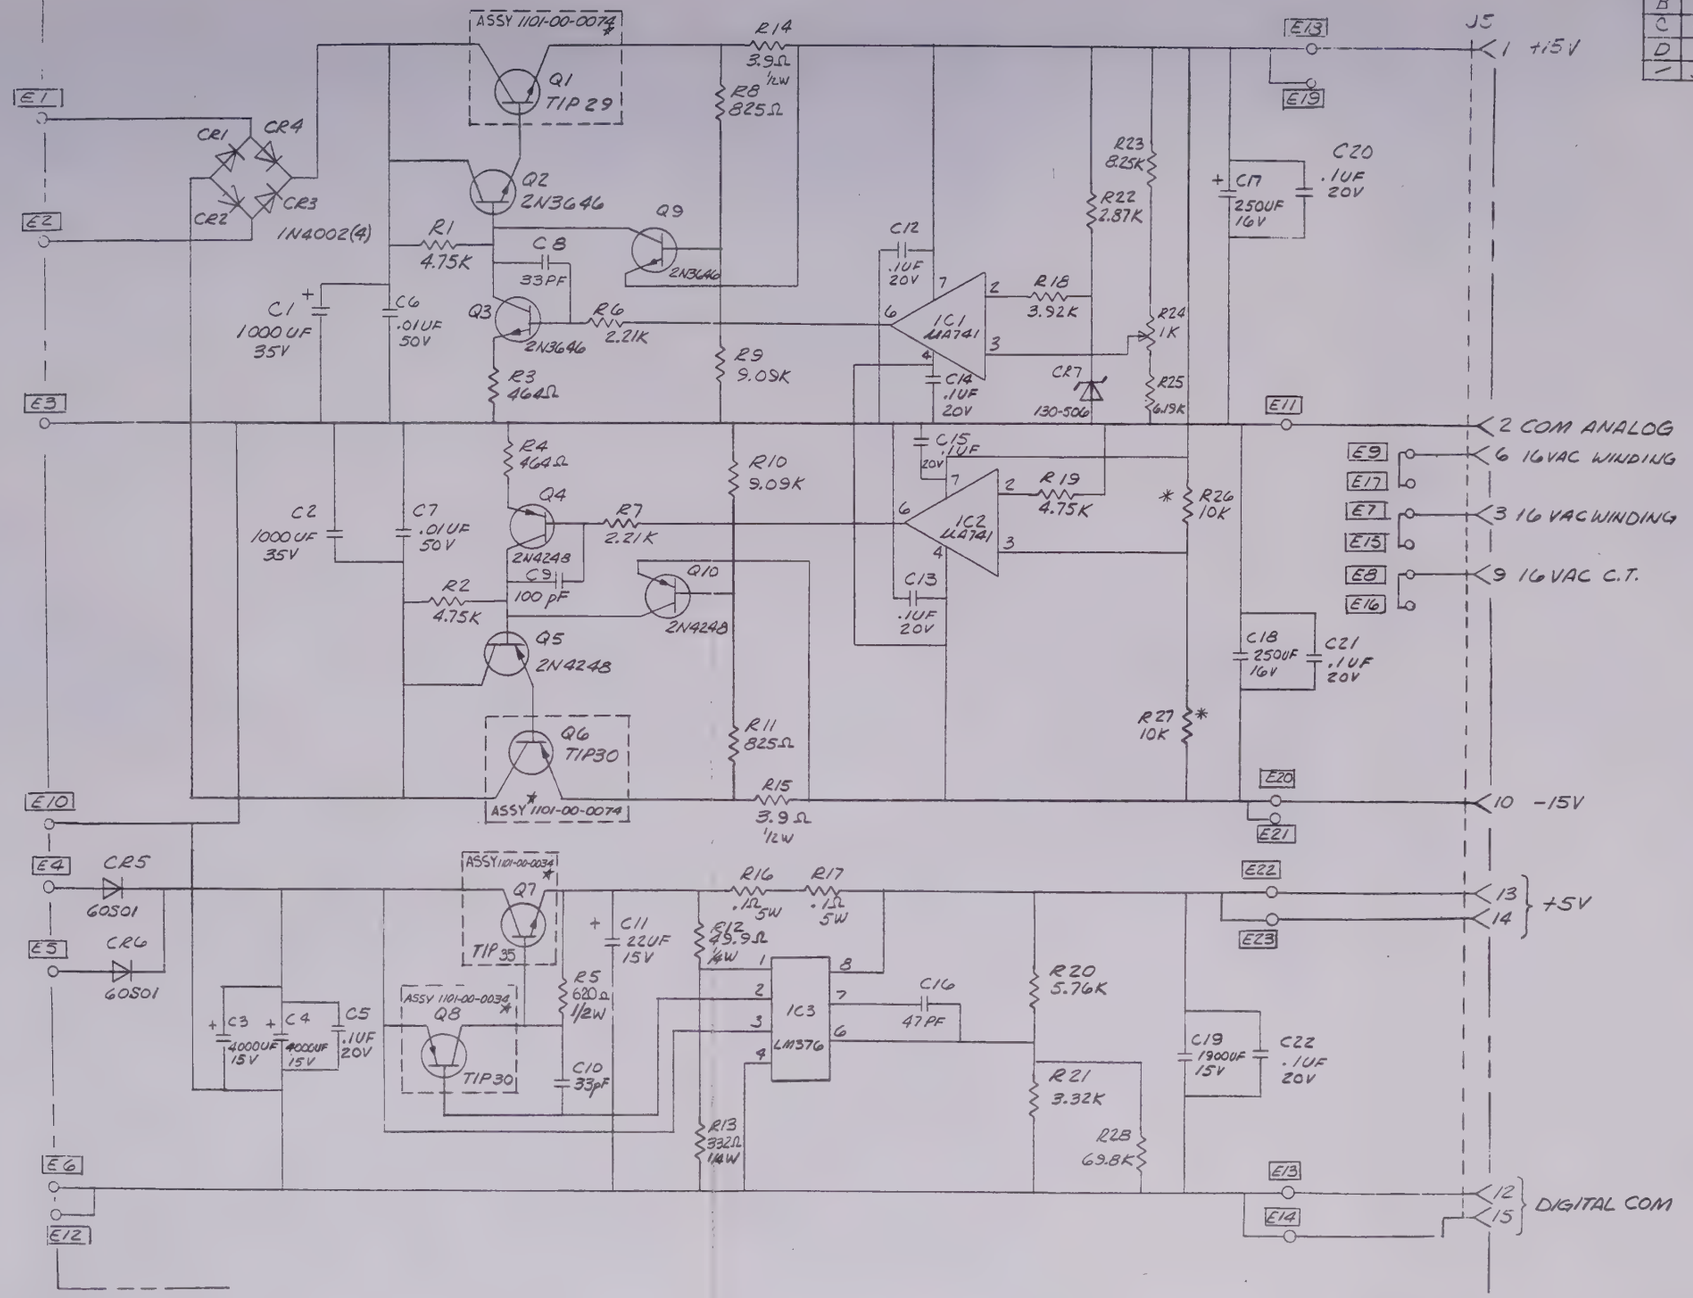

3. ★ ATTACHED TO REAR PANEL HEATSINK BRACKET.
2. * INDICATES MATCHED SET.
1. ALL RESISTORS ARE 1/8W 1%.

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN CL [illegible]	DATE 3/25/74	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL ——	PROJENG [illegible]	4/1/74	TITLE SCHEMATIC POWER SUPPLY A1
	RELEASE APPROV		
FINISH WAVETEK PROCESS ——	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX : .010 ANGLES : 1 XX : .030		
	DO NOT SCALE DWG		MODEL NO. 158/159
	SCALE NONE		DWG NO 0103-00-0108 REV D
	CODE IDENT 23338		SHEET 1 OF 1

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
C	1069	LGC	8/12/76	RPS
D	ECN 1303	RO	6-11-78	RPS
E	ECN 1754	RO	6-20-78	

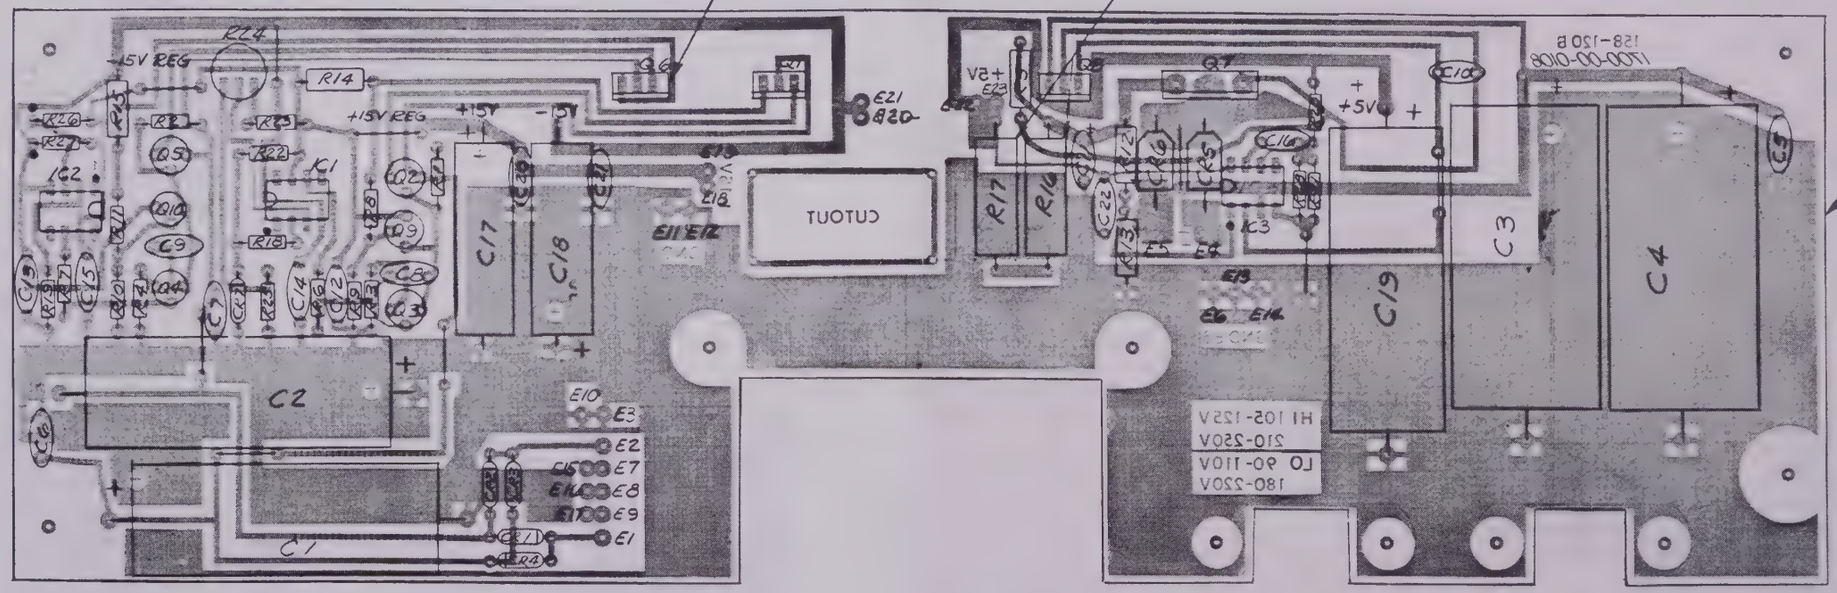

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN C.L. Cox	DATE 4/25/76	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL ——	PROJ ENGR	6/14/74	TITLE PC BOARD ASSY POWER SUPPLY BD
	RELEASE APPROV		
FINISH WAVETEK PROCESS ——	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030		
	DO NOT SCALE DWG		MODEL NO 158/159
	SCALE 2:1		DWG NO. 0101-00-0108 REV E
			CODE IDENT 23338 SHEET 1 OF 1

BRUNING 40-520 15821

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	ASSY DRWG, POWER	0101-00-0108	WVTK	0101-00-0108	1
NONE	SCHEMATIC, POWER	0103-00-0108	WVTK	0103-00-0108	1
C8 C9	CAP, CER, 100PF, 1KV	DD-101 LONG LEAD	CRL	1500-01-0101	2
C6 C7	CAP, CER, MN, .01MF, 50V	CAC02Z5U103Z100A	CORNG	1500-01-0310	2
C12 C13 C14 C15 C20 C21 C22 C5	CAP, CER, MON, .1MF, 50V	CAC03Z5U104Z050A	CORNG	1500-01-0405	8
C10	CAP, CER, 33PF, 1KV	DD-330	CRL	1500-03-3011	1
C16	CAP, CER, 47PF, 1KV	DD-470	CRL	1500-04-7011	1
C1 C2	CAP, ELECT, 1000MF, 35V	39D108G035GL6	SPRAG	1500-31-0212	2
C19	CAP, ELECT, 1900MF, 15V	39D198G015GL4	SPRAG	1500-31-9201	1
C17 C18	CAP, ELECT, 250MF, 16V	500D257G016DF7	SPRAG	1500-32-5101	2
C3 C4	CAP, ELECT, 4000MF, 15V	39D408G015JL4	SPRAG	1500-34-0201	2
C11	CAP, TANT, 22MF, 15V	196D226X9015KA1	SPRAG	1500-72-2601	1
1	POWER	138-120	WVTK	1700-00-0108	1
R24	POT, TRIM, 1K	91AR1K	BECK	4600-01-0209	1
R14 R15	RES, C, 1/2W, 5%, 3.9	RC20GF-3R9	STKPL	4700-25-0399	2
R5	RES, C, 1/2W, 5%, 620	RC20GF621	STKPL	4700-25-6200	1
R6 R7	RES, MF, 1/8W, 1%, 2.21K	RN55D-2211F	TRW	4701-03-2211	2

WAVETEK PARTS LIST	TITLE POWER	ASSEMBLY NO. 1100-00-0108	REV G
		PAGE: 1	

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
R22	RES, MF, 1/8W, 1%, 2.87K	RN55D-2871F	TRW	4701-03-2871	1
R21	RES, MF, 1/8W, 1%, 3.32K	RN55D-3321F	TRW	4701-03-3321	1
R18	RES, MF, 1/8W, 1%, 3.92K	RN55D-3921F	TRW	4701-03-3921	1
R3 R4	RES, MF, 1/8W, 1%, 464	RN55D-4640F	TRW	4701-03-4640	2
R1 R19 R2	RES, MF, 1/8W, 1%, 4.75K	RN55D-4751F	TRW	4701-03-4751	3
R20	RES, MF, 1/8W, 1%, 5.76K	RN55D-5761F	TRW	4701-03-5761	1
R25	RES, MF, 1/8W, 1%, 6.19K	RN55D-6191F	TRW	4701-03-6191	1
R28	RES, MF, 1/8W, 1%, 69.8K	RN55D-6982F	TRW	4701-03-6982	1
R11 R8	RES, MF, 1/8W, 1%, 825	RN55D-8250F	TRW	4701-03-8250	2
R23	RES, MF, 1/8W, 1%, 8.25K	RN55D-8251F	TRW	4701-03-8251	1
R10 R9	RES, MF, 1/8W, 1%, 9.09K	RN55D-9091F	TRW	4701-03-9091	2
R13	RES, MF, 1/4W, 1%, 332	RN60D-3320F	TRW	4701-13-3320	1
R12	RES, MF, 1/4W, 1%, 49.9	RN60D-49R9F	TRW	4701-13-4999	1
R16 R17	RES, WW, 5W, 10%, .1	CP-5	DALE	4702-66-0019	2
R26 R27	RES, SET, 2-10K, 1/8W GTY: 2: 4701-03-1002	142-501-64A	WVTK	4789-00-0019	1
CR7	DIODE	1N4581	MICRO	4801-01-4581	1
CR1 CR2 CR3 CR4	DIODE	1N4002	FAIR	4801-02-0001	4

WAVETEK PARTS LIST	TITLE POWER	ASSEMBLY NO. 1100-00-0108	REV G
		PAGE: 2	

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
CR5 CR6	DIODE	6OS1	IR	4806-02-0060	2
Q2 Q3 Q9	TRANS	2N3646	NSC	4901-03-6460	3
Q10 Q4 Q5	TRANS	2N4248	FAIR	4901-04-2480	3
Q1	TRANS	TIP-29	TI	4902-00-0290	1
Q6 Q8	TRANS	TIP-30	TI	4902-00-0300	2
Q7	TRANS	TIP-35	TI	4902-00-0350	1
IC3	IC	LM376	NSC	7000-03-7600	1
IC1 IC2	IC	LM741CN	NSC	7000-07-4100	2

WAVETEK PARTS LIST	TITLE POWER	ASSEMBLY NO. 1100-00-0108	REV G
		PAGE: 3	

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL	PROJ ENGR		TITLE PARTS LIST POWER
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ± .010 ANGLES ± 1 XX ± .030		
	DO NOT SCALE DWG		MODEL NO 159 / DWG NO 1100-00-0108 / REV G
	SCALE		CODE IDENT 23338 / SHEET 1 OF 1

BISHOP GRAPHICS/ACCUPRESS REORDER NO. A-3694

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	ECN 1368	RO	11-11-97	

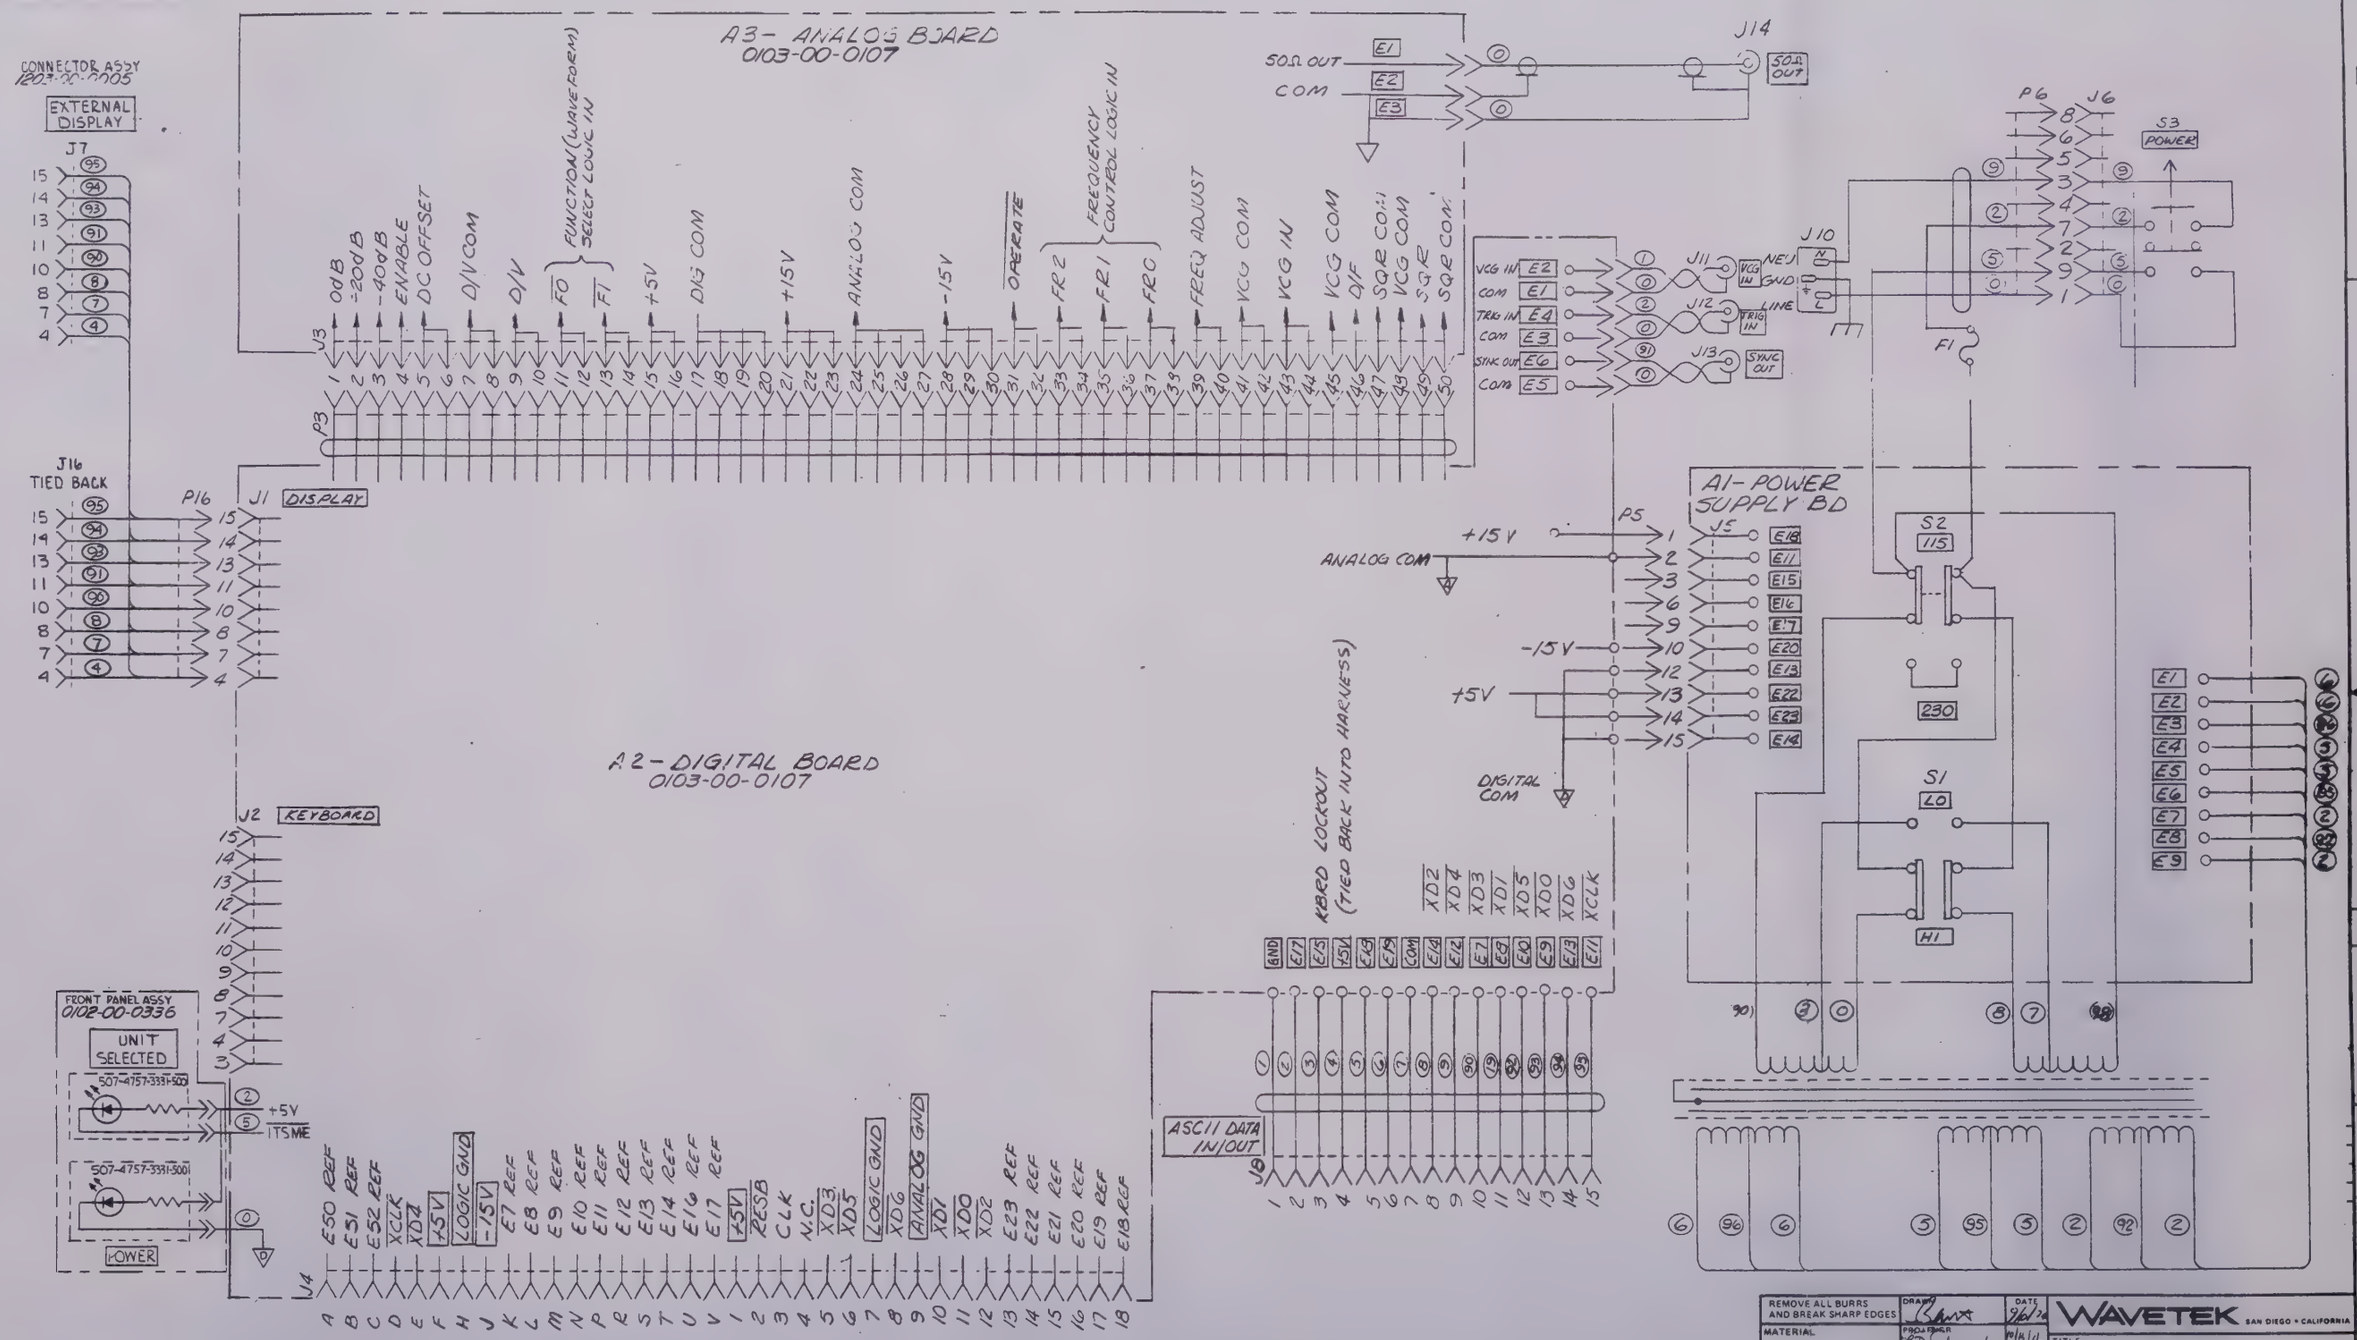

NOTES:
1. ▭ DENOTES ACTUAL LABELING ON UNIT
2. BAR OVER MNEMONIC DENOTES TRUE WHEN LOW
3. ⬭ DENOTES WIRE COLOR PER RESISTOR CODE

REMOVE ALL BURRS AND BREAK SHARP EDGES
MATERIAL
FINISH WAVETEK PROCESS
DRAWN 9/6/94
PROGRAMMER 9/8/94
RELEASE APPROV 1/14/94
TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ±.010 ANGLES ±1 XX ±.030
DO NOT SCALE DWG
SCALE

WAVETEK SAN DIEGO, CALIFORNIA

TITLE: INTERCONNECT DIAGRAM 158 OPTION

MODEL NO. 158/159
DWG NO 0004-00-0081
REV A
CODE IDENT 23338
SHEET 1 OF 1

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

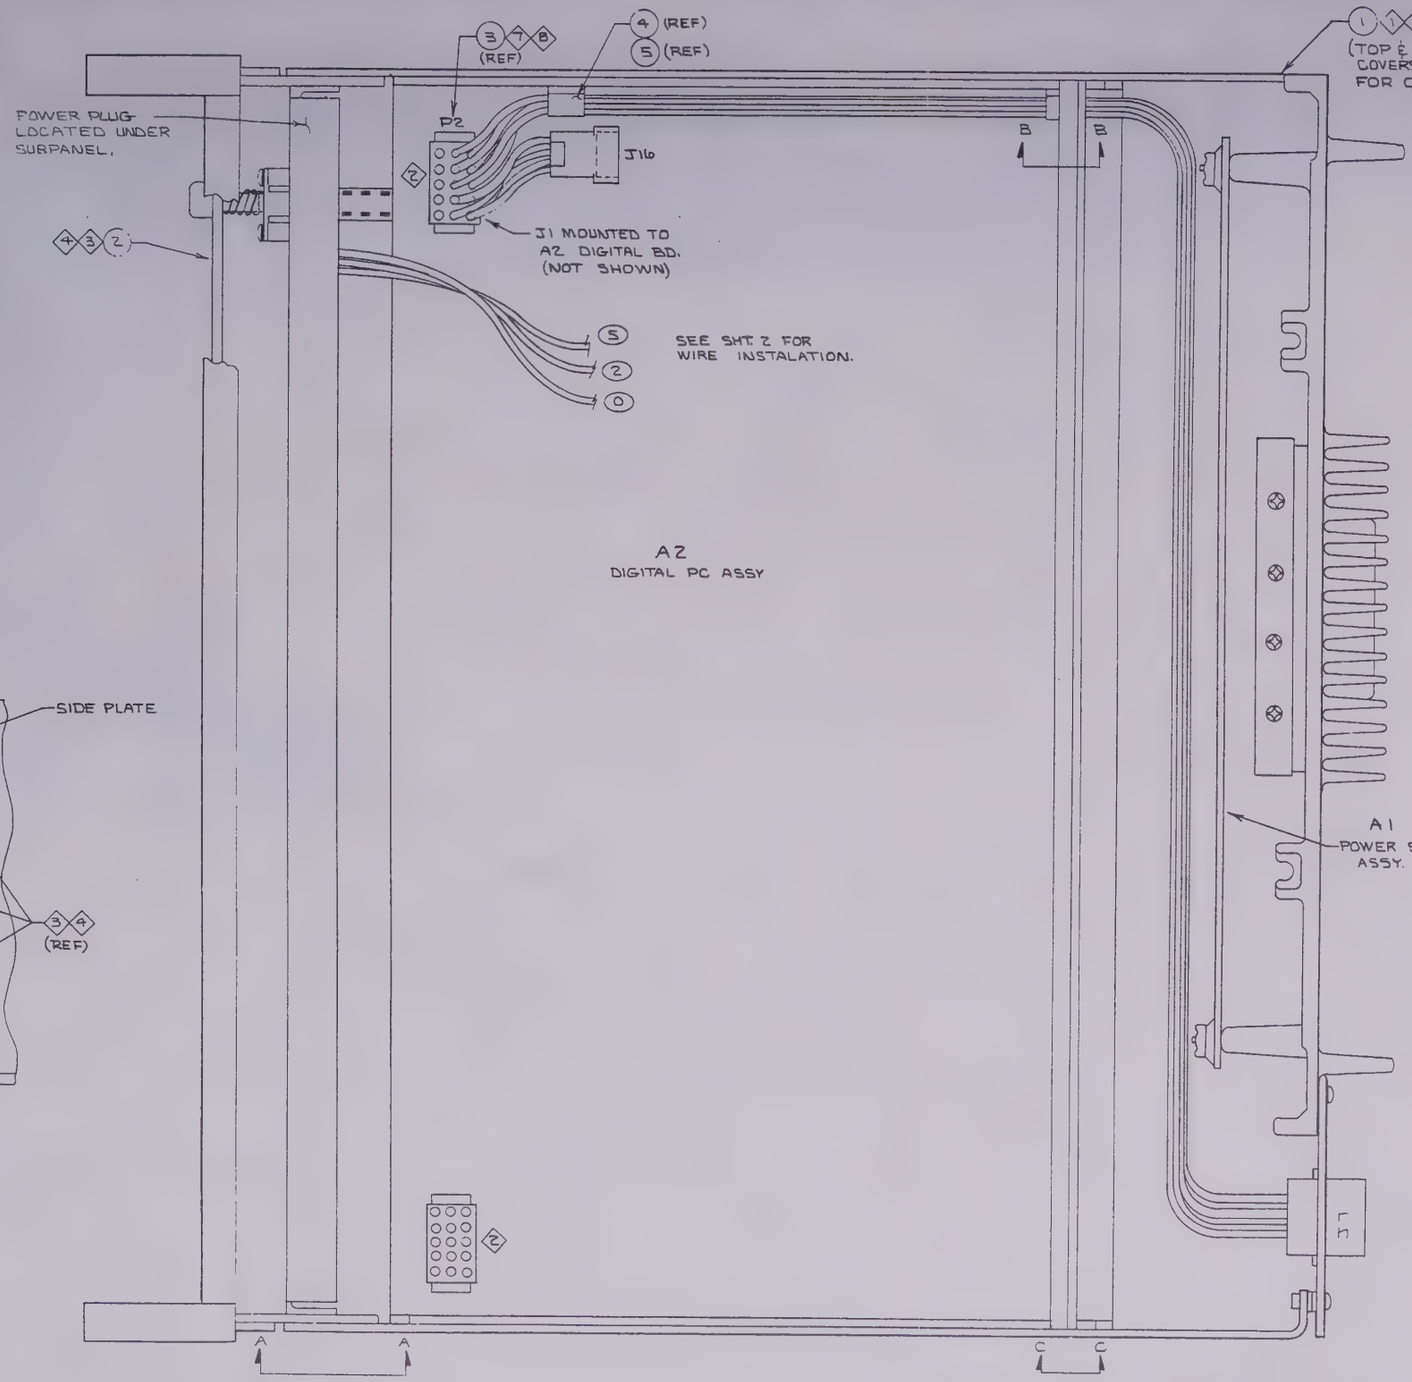

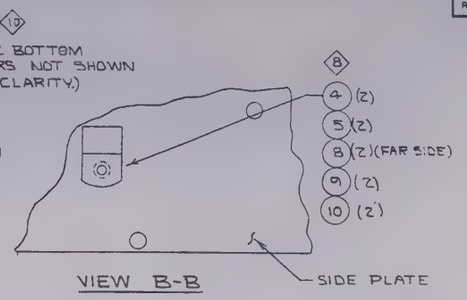

VIEW B-B

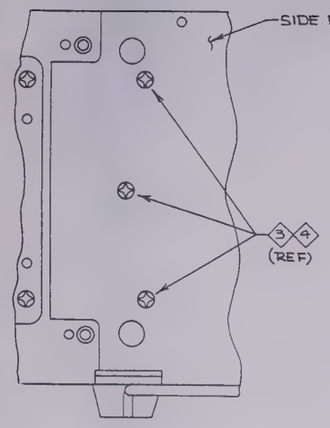

VIEW A-A

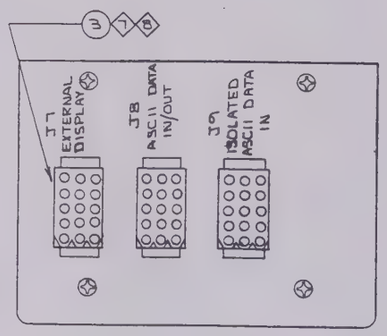

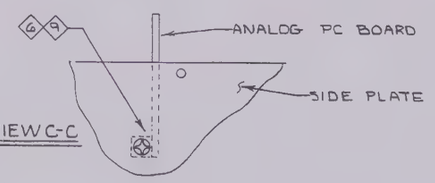

VIEW C-C

3. ⚠ PULL HARDWARE FOR FIELD INSTALATION ONLY.
2. ◇ DENOTES LINE NUMBER FOR MODIFCATION PROCEDURE.
NOTE UNLESS OTHERWISE SPECIFIED 1. ◯ DENOTES WIRE COLOR PER RESISTOR CODE.

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN ADKINS	DATE 10-2-74	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	ENGR	12/13/74	TITLE MODIFICATION DWG 158 OPTION
FINISH WAVETEK PROCESS	RELEASE APPROV JR 12/24/74		
	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030		
	DO NOT SCALE DWG SCALE	MODEL NO. 158	DWG NO. 0102-00-0303 REV
		CODE IDENT 23338	SHEET 1 OF 2

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

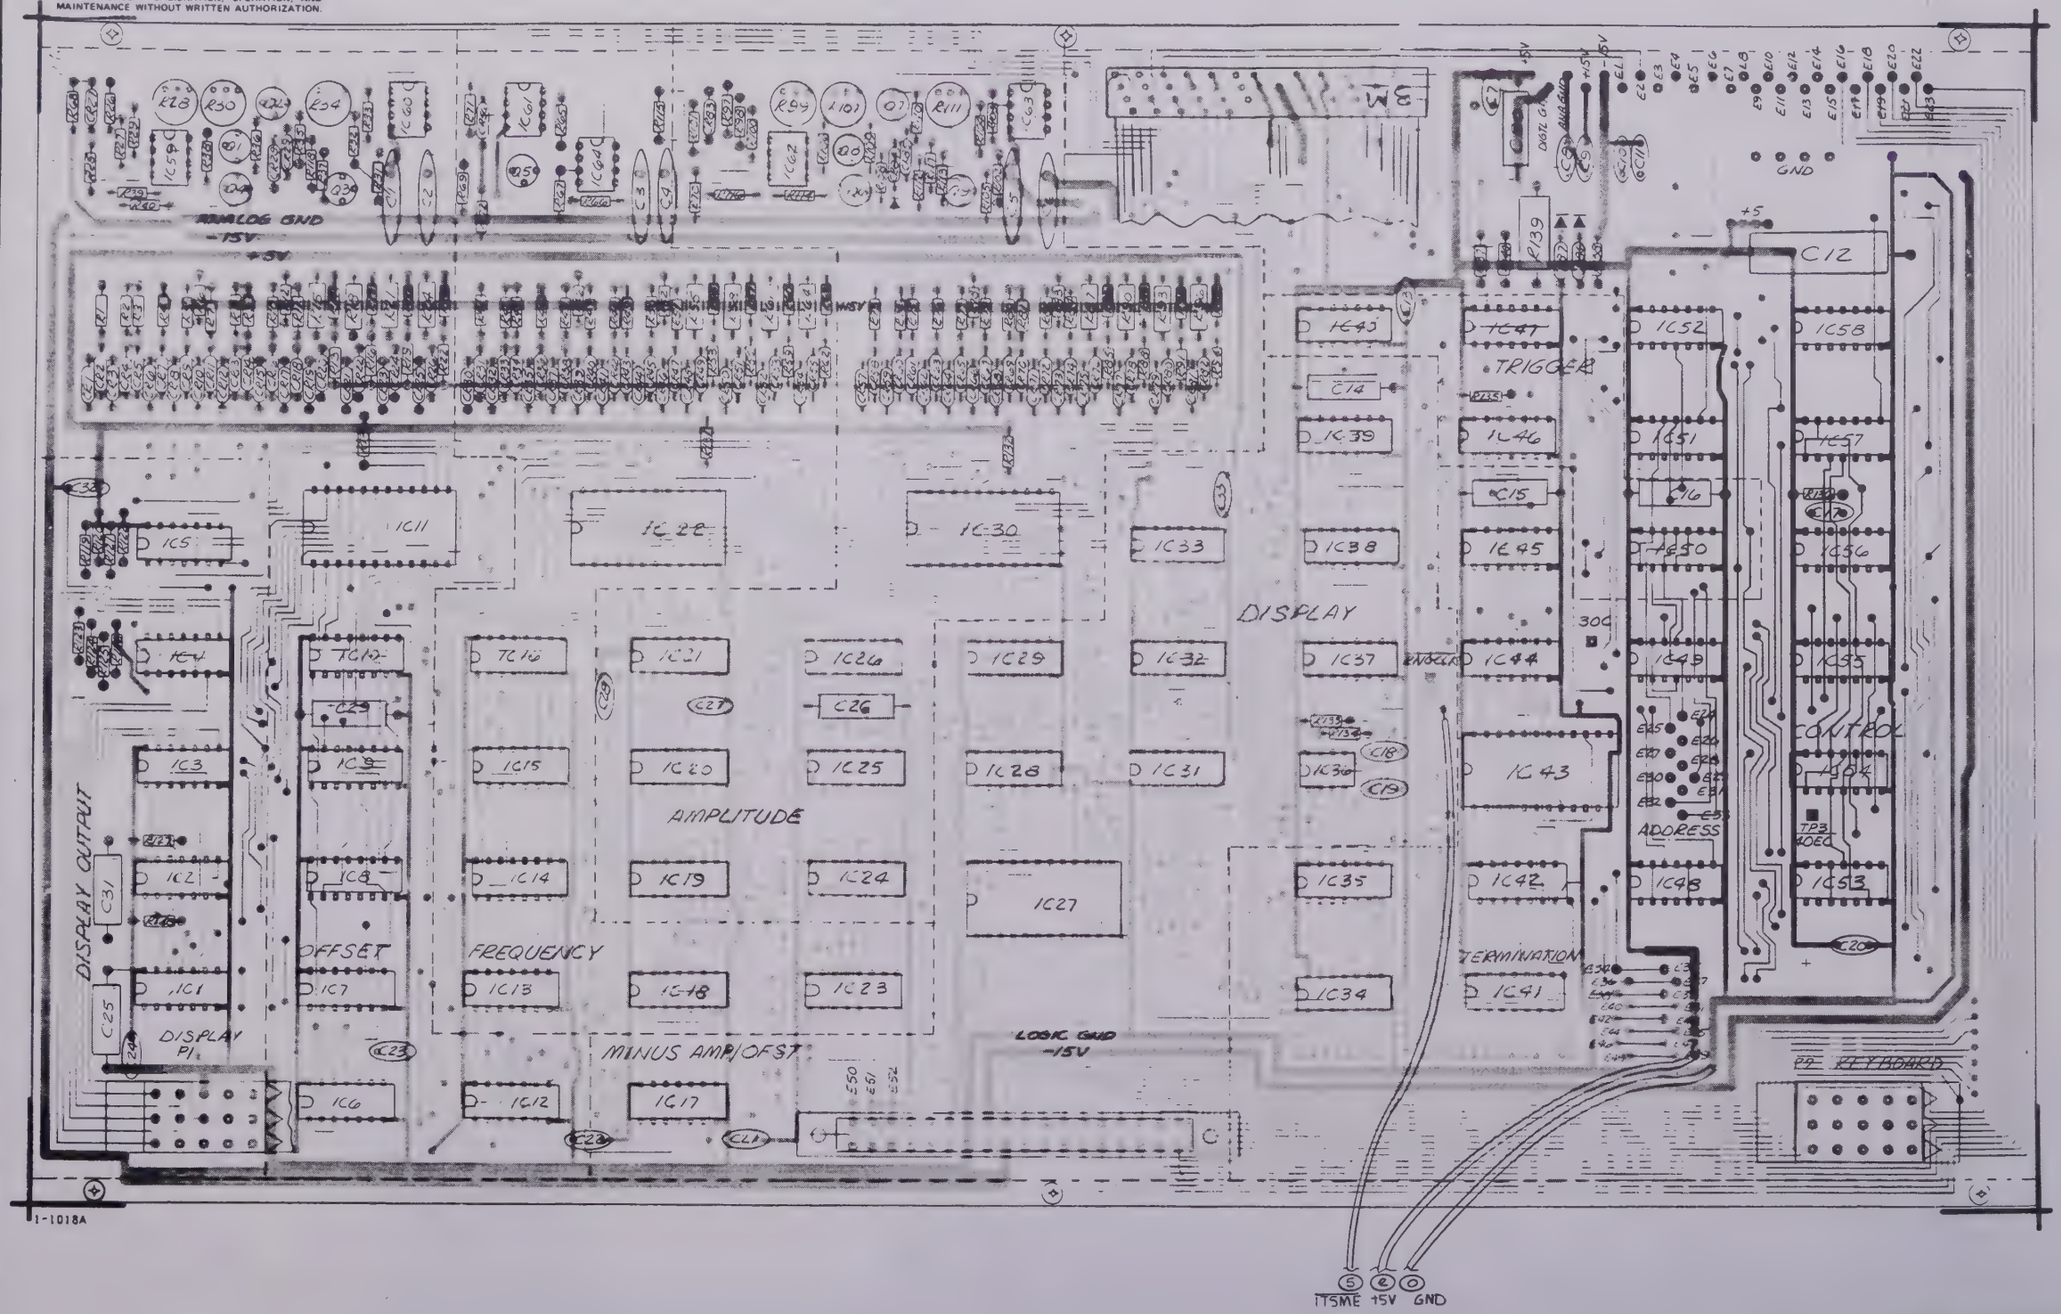

2. ○ DENOTES WIRE COLOR PER RESISTOR CODE

1. ALL DIODES ARE POSITIONED AS SHOWN

NOTE UNLESS OTHERWISE SPECIFIED

SHEET 3 OF 3 IS "A" SIZE MOD. PROC.

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN Barry K	DATE 9-26	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL —	APPROVED [signature]	9/8/94	TITLE MODIFICATION DWG 158 OPTION
FINISH WAVETEK PROCESS —	RELEASE APPROV LPS	12/11/94	
	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX .010 ANGLES ±1 XX .030		
	DO NOT SCALE DWG	MODEL NO 158	DWG NO 0102-00-0303 REV
	SCALE NONE	CODE IDENT 23338	SHEET 2 OF 3

MODIFICATION PROCEDURE

1. REMOVE TOP AND BOTTOM COVERS.

2. DISCONNECT POWER PLUG P6, DISPLAY PLUG P1 AND KEYBOARD PLUG P2.

3. REMOVE FRONT PANEL ASSY 1100-00-0075 AND RETURN TO STOCK.

4. INSTALL FRONT PANEL ASSY 1101-00-0078 AS SHOWN.

5. CONNECT POWER PLUG P6, TO NEW FRONT PANEL ASSY.

6. REMOVE SCREWS AND RAISE ANALOG BOARD TO FACILITATE INSTALLATION OF WIRES TO DIGITAL BOARD.

7. REMOVE BLANK MOLEX CONNECTOR FROM THE EXTERNAL DISPLAY LOCATION ON REAR PANEL AND RETURN TO STOCK.

8. INSTALL CONNECTOR ASSY 1203-00-0005. CONNECT P16 TO J1 ON THE A2 DIGITAL PC ASSY. INSTALL MOLEX TO EXTERNAL DISPLAY LOCATED ON THE REAR EXTENDER AS SHOWN.

9. LOWER ANALOG PC ASSY AND INSTALL SCREWS.

10. INSTALL TOP AND BOTTOM COVERS.

DWG NO.	REV
0102-00-0303	

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	ASSY DRWG, 158 MOD	0102-00-0303	WVTK	0102-00-0303	1
3	CABLE ASSY	158-039	WVTK	1203-00-0005	1
NONE	CABLE CLAMP	835	SMITH	2800-00-0010	2
NONE	RETAINER, SPRING	D-191	WEKSR	2800-09-0007	2

WAVETEK PARTS LIST	TITLE MODIFICATION KIT	ASSEMBLY NO. 1101-00-0044 PAGE: 1	REV A

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: PARTS LIST MODIFICATION KIT
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ± .010 ANGLES ±1 .XX ± .030		MODEL NO 158 / DWG NO 1101-00-0044 / REV A
	DO NOT SCALE DWG		CODE IDENT 23338 / SHEET 1 OF 1
	SCALE		

BISHOP GRAPHICS/ACCUPRESS REORDER NO. A-5884

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	ECN 1160	RS	12/4/74	
B	ECN 1315	[illegible]	6-20-75	

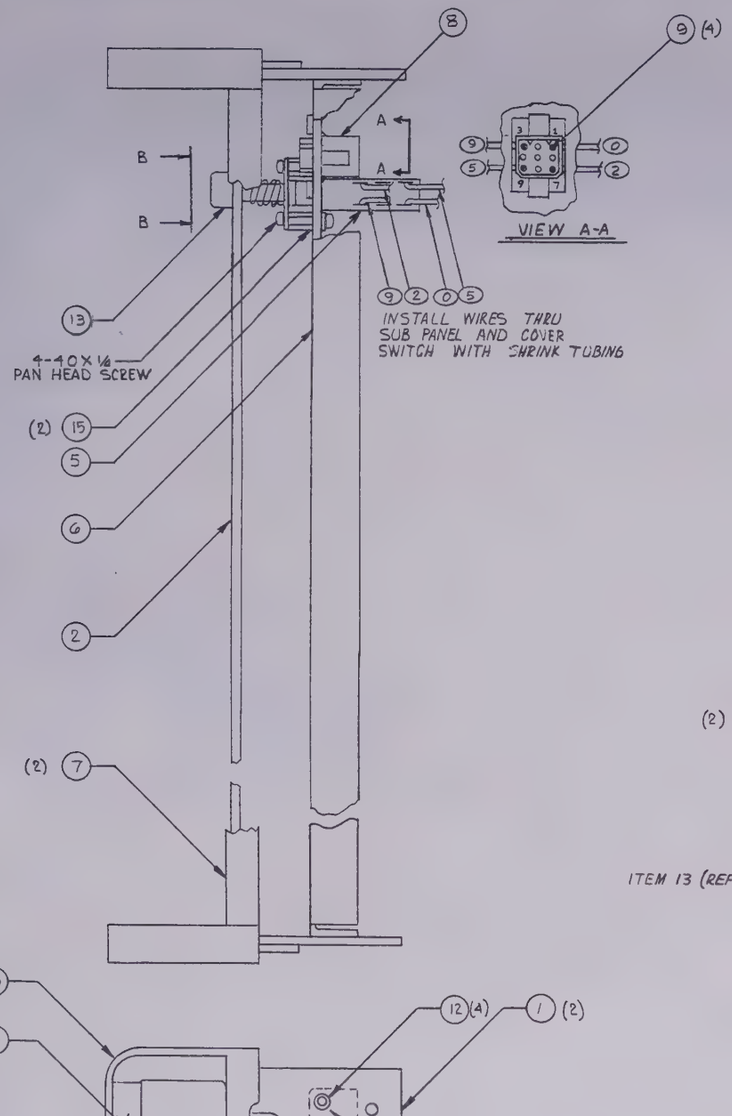

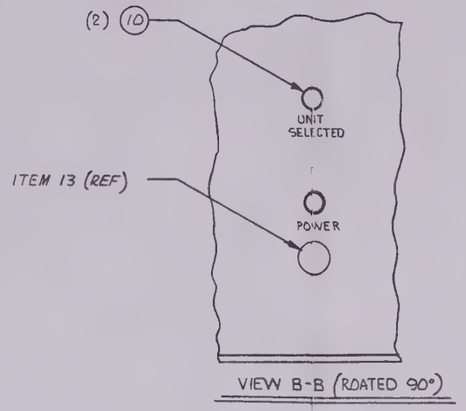

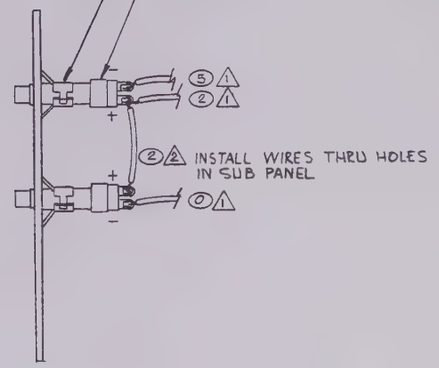

3. ⬭ DENOTES WIRE COLOR PER RESISTOR CODE
2 CUT WIRE TO A LENGTH OF 3"
1 CUT WIRES TO A LENGTH OF 16" AND STRIP ENDS

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN BARNETT	DATE 9/6	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ MGR [illegible]	10/4	TITLE FRONT PANEL ASSY- 158 OPTION
	RELEASE APPROV [illegible]	12/12/74	
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030		
	DO NOT SCALE DWG		MODEL NO 158 / DWG NO. 0102-00-0336 / REV B
	SCALE FULL		CODE IDENT 23338 / SHEET 1 OF 1

0102-00-0336

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	ASSY DRWG, FT PNL	0102-00-0336	WVTK	0102-00-0336	1
6	PANEL, SUB	158-323	WVTK	1400-00-0723	1
1 1A	BRKT	158-324	WVTK	1400-00-0733	2
15 15A	STANDOFF	013-003-2	WVTK	1400-00-2503	2
3 3A	HANDLE, R/A FROM: 1400-00-3561	147-364	WVTK	1400-00-3589	2
4 4A	TRIM, HANDLE REF: 3200-06-0006	147-345	WVTK	1400-00-3619	2
2	PANEL, FT	158-326	WVTK	1400-00-5570	1
7	TRIM REF: 3200-06-0005	1400-00-7019	WVTK	1400-00-7019	2
8	PLUG, 9PIN	03-06-2091	MOLEX	2100-02-0011	1
11 11A	CONN, LAMP	515-0074	DILCO	2100-03-0024	2
NONE	PIN, MALE	02-06-2103	MOLEX	2100-05-0003	4
NONE	LAMP CARTRIDGE	507-4757-3331-300	DILCO	2400-02-0016	2
14 14A	CLIP	515-0051	DILCO	2800-36-0003	2
5	SWITCH ASSY PB	157-422	WVTK	5103-00-0011	1
13	BUTTON	J-52305-BLACK	CRL	5103-04-0003	1

WAVETEK PARTS LIST	TITLE FT PANEL ASSY	ASSEMBLY NO. 1101-00-0078 PAGE: 1	REV B

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: PARTS LIST FT PANEL ASSY
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1 XX ±.030		
	DO NOT SCALE DWG		MODEL NO 158 · DWG NO 1101-00-0078 · REV B
	SCALE		CODE IDENT 23338 · SHEET 1 OF 1

BISHOP GRAPHICS/ACCUPRESS REORDER NO A-3894

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

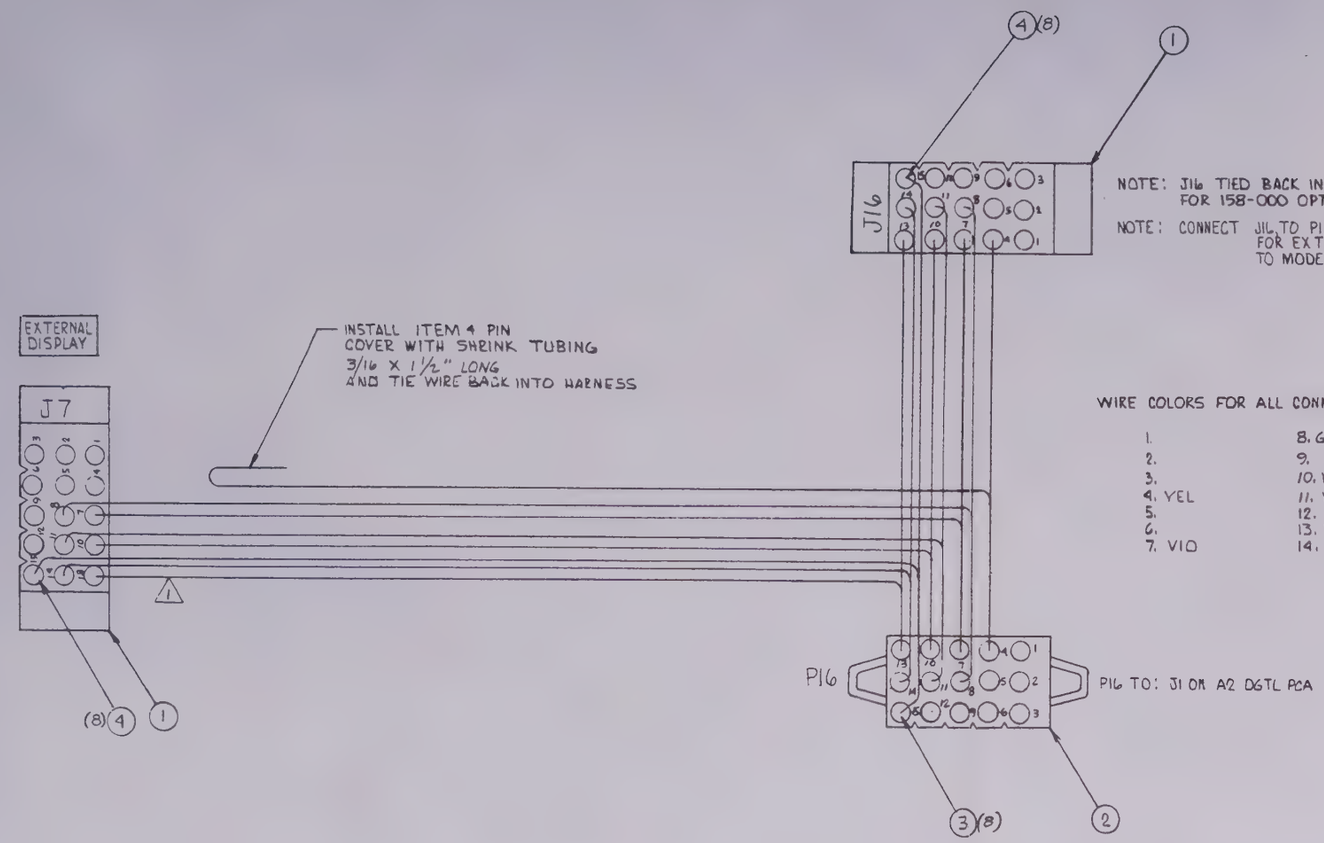

NOTE: J16 TIED BACK INTO HARNESS FOR 158-000 OPTION

NOTE: CONNECT J16 TO P1 ON A5 DISPLAY PCA FOR EXTERNAL DISPLAY OPTION TO MODEL 159.

WIRE COLORS FOR ALL CONNECTORS

1.	8. GRY	15. WHT/GRN
2.	9.	
3.	10. WHT/BLK	
4. YEL	11. WHT/BRN	
5.	12.	
6.	13. WHT/ORN	
7. VIO	14. WHT/YEL	

3. TIE WIRES USING SMALL CABLE TIE 23M AS REQ

△2 CUT WIRES TO A LENGTH OF 3.0 INCHES

△1 CUT WIRES TO A LENGTH OF 28.5 INCHES

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN [illegible]	DATE 9/10	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL	ENGR [illegible]	12/4/14	TITLE CONNECTOR ASSY- EXT. DISPLAY
FINISH WAVETEK PROCESS	RELEASE APPROV [illegible]	12/17/14	
	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ±.010 ANGLES ±1 XX ±.030		
	DO NOT SCALE DWG	MODEL NO 158	DWG NO 120-00-0005 REV
	SCALE	CODE IDENT 23338	SHEET 2 OF 2

APPENDIX A
GPIB OPTION 005

A.1 MODEL 159 GPIB

Option 159-005 (General Purpose Interface Bus) is compatible with IEEE Standard 488-1975 and 1978 (for Model 159 purposes, the IEEE 488-1975 and 1978 standards are the same). Previous names, including IEC and HP-IB, always refer to the GPIB.

The GPIB Option 159-005 implements Acceptor Handshake (AH), Listen (L), Remote Enable (REN) and Go To Local (GTL). Group Execute Trigger (GET) is not implemented. No provisions for Service Request or Polling have been made. (The SRQ and EOI lines are not used.)

A.1.1 REN Function

The GPIB equipped generator will be in a Remote Only condition if the GPIB option card is addressed to Listen while the REN line is set. (Remote Ony implies that the generator's keyboard will be disabled). Either a Go To Local (GTL) command or resetting the REN line will enable the generator's keyboard.

A.1.2 GPIB Listen Address

The GPIB listen address is independent of the generator unit address. The GPIB card provides the controller-to-instrument transfer of data when ever the GPIB addressed data and instrument GPIB address agree. The GPIB card, when addressed, translates the GPIB data into Wavetek synchronous bus - data (figure A-1). The Wavetek bus then distributes data both to the rear panel for other possible units and also to the main board of this generator. The instrument unit address (not GPIB address) is hardwire jumpered to be from 1 through 9. An incoming unit address, ASCII code of G1 through G9, selects the particular 159 instrument to receive new programming information.

Unless otherwise specified, GPIB options are delivered with an address of "(quote mark) for the HP9830 controller (device 02 for the HP9825 and Tektronix 4051 controllers and 34 for the Commodore PET controller. See appendix A for possible addresses). This address can be changed by the switches of component U12A on the GPIB option card.

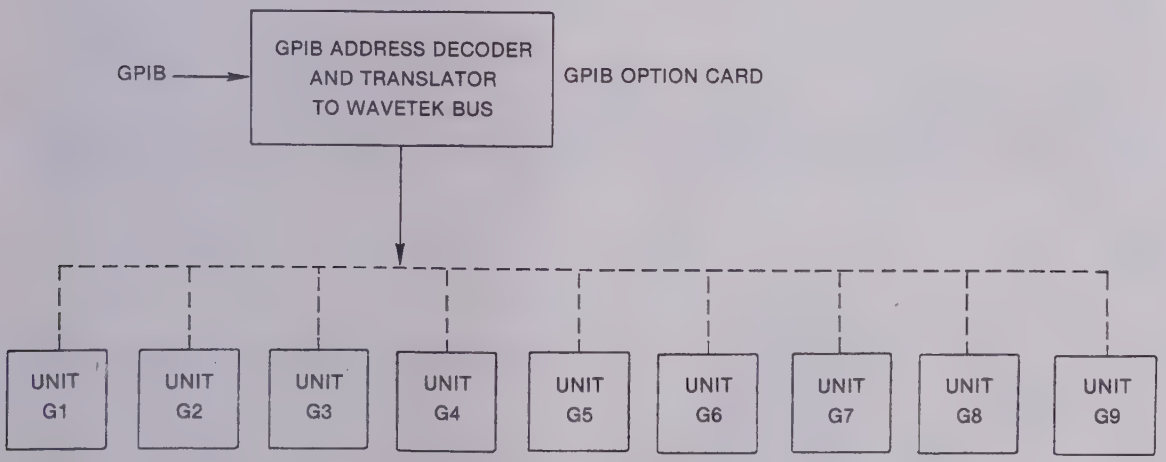

Figure A-1. Wavetek Generators with Unit Address

A.1.3. Changing GPIB Address

Remove the top cover of the 159 and locate the vertically mounted option card at the front of the generator. It is not really necesasary to remove the card to make visual inspections or changes to the GPIB address selector, component U12A. A dextrous hand and an insulated narrow tool (e.g., an orange stick or tuning wand) is all that is necessary for changing the GPIB address. However, if you desire greater access, remove the screws at both ends of the mounting bar and remove the card.

The five switches of S1 (figure A-2) correspond to the lower five data I/0 lines of the GPIB: switch 1 = DIO1, switch 2 = DIO2, etc. All legal listen addresses are listed in table A-1. Set the switches to 0 or 1 as indicated for the desired addresses.

A.1.4 Unit Address

Unless otherwise specified, the Model 159 is delivered with a unit address of 1 (this is not the GPIB address). The merely inspect for the proper unit address, the frontpanel keyboard and display may be used. By pressing UNIT followed by a number entry of 0 through 9, ventually the UNIT SELECTED LED will light. This indicated that this particular instrument, unit (figure A-1), is selected for programming. Once a unit is selected, all programming that reaches the Wavetek ASCII bus is for that unit; the unit designator need not be repeated unless a different unit is desired. The unit address may similarly be determined via remote programming and the ASCII G code.

The unit address may be changed by repositioning the unit address jumper on the digital board of the generator.

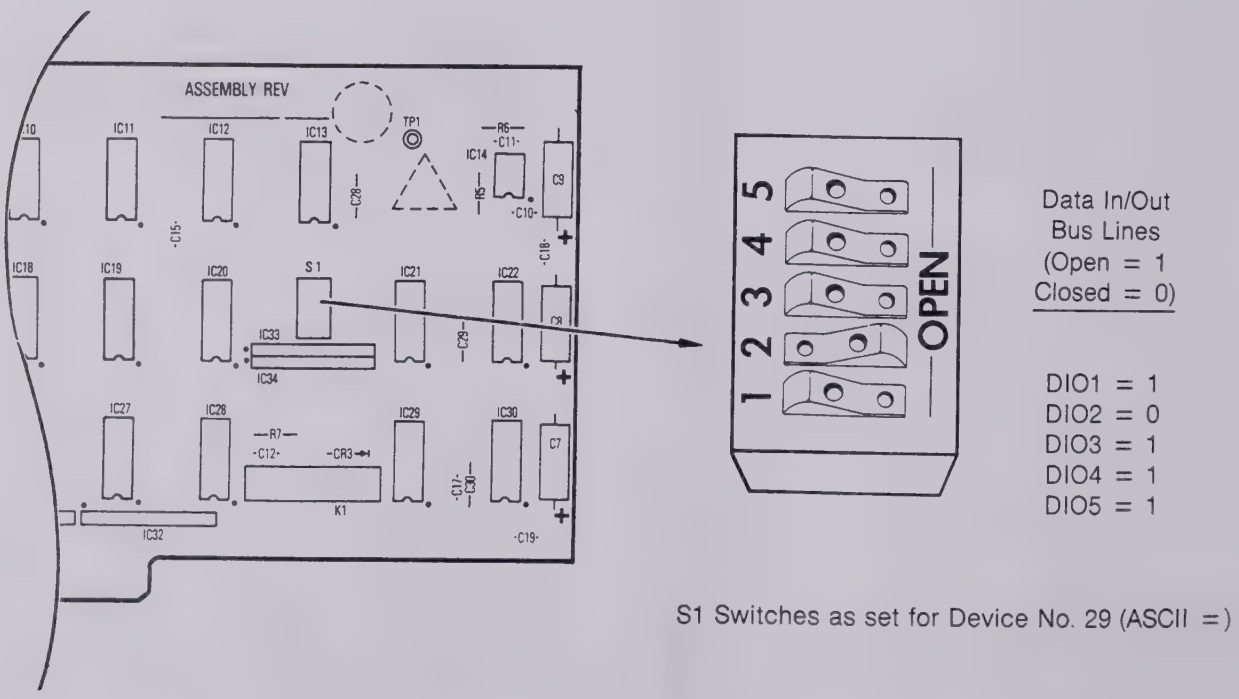

Figure A-2. GPIB Address Selector on the GPIB Option Card.

A.1.5 Changing Unit Address

Remove top and bottom covers of generator. Remove screws from both ends of the analog board front mounting bar (top horizontal board). Rotate and secure analog board in an UP position. Locate address pads E24 through E33. (See figure A-3.) A soldering iron is required to move the jumper on the digital board.

Jumper E29 to E24 for unit address of 1.
Jumper E29 to E25 for unit address of 2.
Jumper E29 to E26 for unit address of 3.
Jumper E29 to E27 for unit address of 4.
Jumper E29 to E28 for unit address of 5.
Jumper E29 to E30 for unit address of 6.
Jumper E29 to E31 for unit address of 7.
Jumper E29 to E32 for unit address of 8.
Jumper E29 to E33 for unit address of 9.

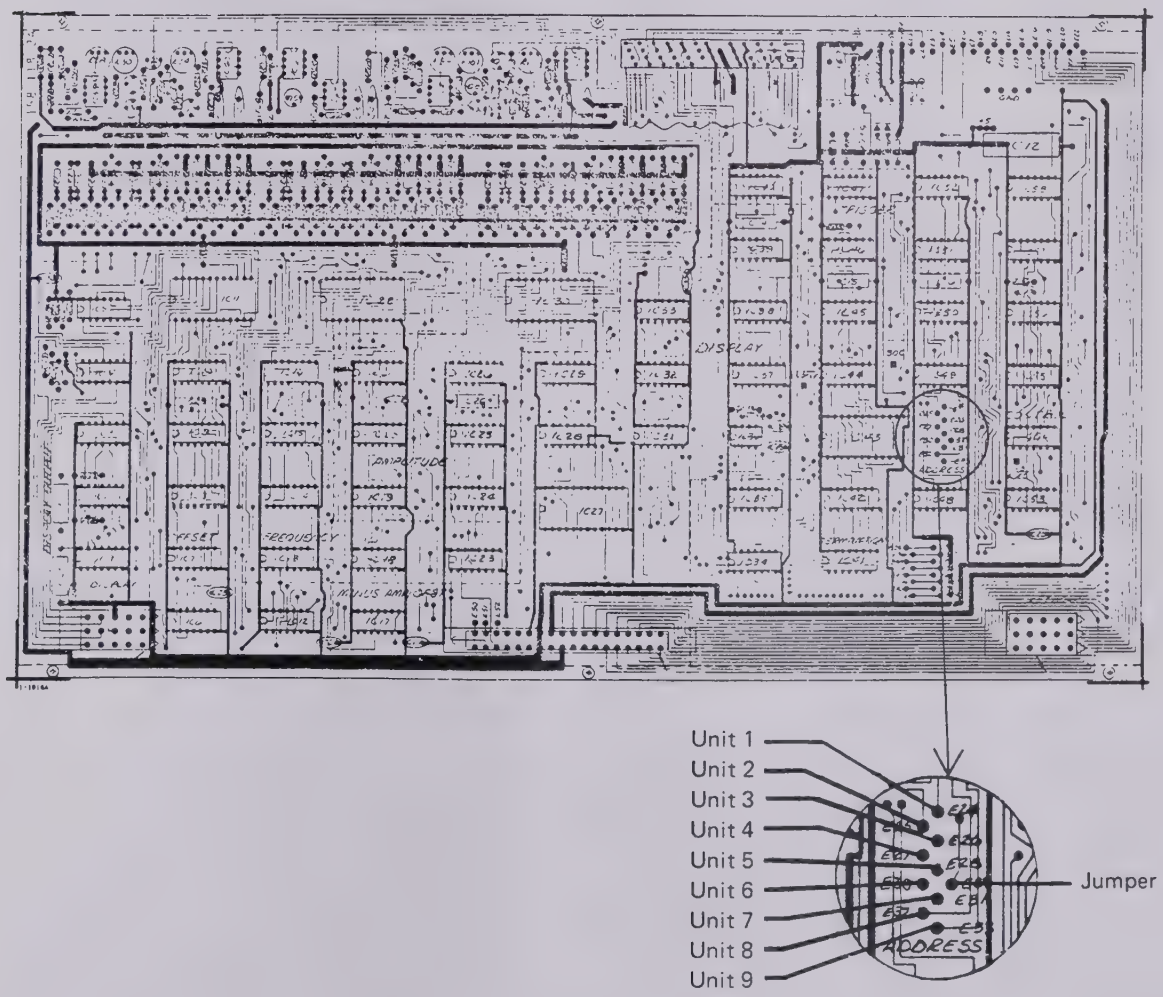

Figure A-3. Model 158/159 Digital Board (Top View)

Table A-1. General Purpose Interface Bus Address

HP9825 TEK4051	HP9830	Primary Listen Address								
		Decimal Value	DIO Bus							
			8	7	6	5	4	3	2	1
Device Ø	SP	32	0	0	1	0	0	0	0	0
Device 1	!	33	0	0	1	0	0	0	0	1
Device 2	"	34	0	0	1	0	0	0	1	0
Device 3	#	35	0	0	1	0	0	0	1	1
Device 4	$	36	0	0	1	0	0	1	0	0
Device 5	%	37	0	0	1	0	0	1	0	1
Device 6	&	38	0	0	1	0	0	1	1	0
Device 7	'	39	0	0	1	0	0	1	1	1
Device 8	(	4Ø	0	0	1	0	1	0	0	0
Device 9	)	41	0	0	1	0	1	0	0	1
Device 1Ø	*	42	0	0	1	0	1	0	1	0
Device 11	+	43	0	0	1	0	1	0	1	1
Device 12	,	44	0	0	1	0	1	1	0	0
Device 13	-	45	0	0	1	0	1	1	0	1
Device 14	.	46	0	0	1	0	1	1	1	0
Device 15	/	47	0	0	1	0	1	1	1	1
Device 16	0	48	0	0	1	1	0	0	0	0
Device 17	1	49	0	0	1	1	0	0	0	1
Device 18	2	5Ø	0	0	1	1	0	0	1	0
Device 19	3	51	0	0	1	1	0	0	1	1
Device 2Ø	4	52	0	0	1	1	0	1	0	0
Device 21	5	53	0	0	1	1	0	1	0	1
Device 22	6	54	0	0	1	1	0	1	1	0
Device 23	7	55	0	0	1	1	0	1	1	1
Device 24	8	56	0	0	1	1	1	0	0	0
Device 25	9	57	0	0	1	1	1	0	0	1
Device 26	:	58	0	0	1	1	1	0	1	0
Device 27	;	59	0	0	1	1	1	0	1	1
Device 28	<	6Ø	0	0	1	1	1	1	0	0
Device 29	=	61	0	0	1	1	1	1	0	1
Device 3Ø	>	62	0	0	1	1	1	1	1	0
Unlisten	?	63	0	0	1	1	1	1	1	1
						5	4	3	2	1
						Switch Sections				

NOTE: Unlisten (?) cannot be used as an address.

A.2 PROGRAM EXAMPLE USING COMMODORE PET CONTROLLER

This program demonstrates the Model 159 only. Other instruments may be left (with power on) connected to the bus provided none of them have the GPIB address on "1". The controller is the Commodore PET with 8K memory.

Display the 159 output on an oscilloscope triggering externally from the 159 SYNC OUT.

Run the program as outlined in the following steps:

1. Turn the PET on (power switch is at the left rear of the PET).
2. Insert the tape cartridge into the tape drive.
3. Type:

   LOAD "DEMO 159"

   Press RETURN.
4. The PET will instruct you to press PLAY on the tape drive. The tape will advance and load the program.
5. When "READY" and flashing "BASIC" appear, type:

   RUN

   Press RETURN.
6. The program is now running. The flashing "BASIC" indicates that the program is finished. The program will normally terminate (exit) itself upon its conclusion.

NOTES:

1. To terminate a program immediately, press STOP. To restart a program, type:

   RUN

   Press RETURN.
2. In loading (searching) for a particular program, the tape will only advance forward. You must rewind the tape to load a program that has been passed.
3. The PET is much slower than the Model 159.

```
1Ø PRINT"159 DEMO"
2Ø REM 28 JAN '8Ø
3Ø REM 159 ADDRESS SET TO 1
4Ø OPEN 2,33
5Ø REM UNIT NUMBER IS ONE
6Ø PRINT#2,"G1"
7Ø REM INITIALIZE
8Ø PRINT#2,"F1ØØE3A999EØDØBØCØH"
9Ø TI$="ØØØØØØ"
95 IFTI<6ØGOTO95
1ØØ FORC=ØTO3
11Ø PRINT#2"C",C
12Ø TI$="ØØØØØØ"
125 IFTI<6ØGOTO125
13Ø NEXTC
14Ø PRINT#2,"CØ"
15Ø REM FREQUENCY***
16Ø FORF=1ØØTO95ØSTEP25
```

```
 17Ø PRINT#2,"F",F
 18Ø TI$="ØØØØØØ"
 185 IFTI<1ØGOTO185
 19Ø NEXTF
 2ØØ FORF=95ØTO1ØØSTEP-25
 21Ø PRINT#2,"F",F
 22Ø TI$="ØØØØØØ"
 225 IFTI<1ØGOTO225
 23Ø NEXTF
 24Ø REM AMPLITUDE ***
 25Ø FORA=999TO-951STEP-5Ø
 26Ø REM 3 DIGITS FOR AMPLITUDE
 27Ø IFABS(A)<1ØTHENPRINT#2,"AØØ",A
 28Ø IFABS(A)>=1ØANDABS(A)<1ØØTHENPRINT#
2,"AØ",A
 29Ø IFABS(A)>=1ØØTHENPRINT#2,"A",A
 3ØØ TI$="ØØØØØØ"
 3Ø5 IFTI<1ØGOTO3Ø5
 31Ø NEXTA
 32Ø FORA=-951TO499STEP5Ø
 33Ø IFABS(A)<1ØTHENPRINT#2,"AØØ",A
 34Ø IFABS(A)>=1ØANDABS(A)<1ØØTHENPRINT#
2,"AØ",A
 35Ø IFABS(A)>=1ØØTHENPRINT#2,"A",A
 36Ø TI$="ØØØØØØ"
 365 IFTI<1ØGOTO365
 37Ø NEXTA
 38Ø REM D C  OFFSET **
 39Ø FORD=ØTO25ØSTEP25
 4ØØ REM 3 DIGITS FOR AMPLITUDE
 41Ø REM A SUBROUTINE USED THIS EXAMPLE
 42Ø GOSUB44Ø
 43Ø GOTO5ØØ
 44Ø REM 3 DIGIT ROUTINE
 45Ø IFABS(D)<1ØTHENPRINT#2,"DØØ",D
 46Ø IFABS(D)>=1ØANDABS(D)<1ØØTHENPRINT#
2,"DØ",D
 47Ø IFABS(D)>=1ØØTHENPRINT#2,"D",D
 48Ø TI$="ØØØØØØ"
 485 IFTI<1ØGOTO485
 49Ø RETURN
 5ØØ NEXTD
 51Ø FORD=25ØTO-25ØSTEP-25
 52Ø REM 3 DIGIT ROUTINE
 53Ø GOSUB44Ø
 58Ø NEXTD
 59Ø REM TRIGGERED MODE W/TRIG'S **
 6ØØ FORI=1TO1ØØØ
 61Ø PRINT#2,"Bi"
 62Ø NEXTI
 63Ø PRINT#2,"F1ØØE3A999EØDØBØCØH"
```

A.3 PROGRAMMING EXAMPLE USING HP 9830 CONTROLLER

```
100  REM PROGRAM DEMONSTRATES USE OF WAVETEK MODEL 158-159 GENERATOR
110  REM ASSUMES MODEL 30 CALCULATOR WITH EXTENDED I/O
120  REM 9820 AND 21 CALCULATORS USE FORMAT B AND WBYTE CMD COMMANDS
130  REM
140  REM UNIT IS ADDRESSED BY A CMD "?U>", "G1"
150  CMD "?U>", "G1"
160  REM WHERE THE FIRST GROUP SELECTS H/P BUS (UNIT 13) UNLISTENS (?),
170  REM THEN SELECTS CALCULATOR TO BE TALKER, > IS ADDRESSED AS A LISTENER
180  REM SECOND GROUP SELECTS UNIT 1 ATN IS SET FOR FIRST GROUP, RESET FOR SECOND
190  REM A1 IS THE UNIT NUMBER; 13 FOR H-P INTERFACE BUS
200  A1=13
210  REM
220  REM AMPLITUDE MAY BE DRIVEN BY;
230  A=5
240  OUTPUT (A1, 250)A;
250  FORMAT "A", E9.2
260  REM  SEMICOLON INHIBITS CR, LF.
270  REM
280  REM FREQUENCY MAY BE DRIVEN BY;
290  F=1234567
300  OUTPUT (A1,310)F;
305  REM USE OF 1000 FORMAT SPECIFICATION DELETES LEADING BLANKS
310  FORMAT "F",E1000.2
320  REM
330  REM OFFSET MAY BE DRIVEN BY;
340  O=1
350  OUTPUT (A1,360)O;
360  FORMAT "D",F6.2
370  REM NOTE THAT OFFSET DOES NOT HAVE A MULTIPLIER DIGIT
380  REM
390  REM FUNCTION AND MODE ARE DRIVEN BY;
400  OUTPUT (A1,*)"B0 C0";
410  REM WOULD SELECT MODE (B) 0, CONTINUOUS, FUNCTION (C) 0 SIN. .
420  REM LEGAL MODE VALUES ARE 0,1,2: FUNCTION INCLUDES 0,1,2,3. .
430  REM OUTPUT IS ENABLED BY;
440  OUTPUT (A1,*)"H"
450  REM WHERE H ENABLES OUTPUT OF GENERATOR TO CONNECTOR. . .
460  REM SENDING AN "I" WILL DISCONNECT GENERATOR OUTPUT.
470  REM
480  REM SPECIAL CHARACTERS CONTROL H-P INTERFACE BUS. . .
490  REM ATN IS ENABLED BY OUTPUT (13,500)256;
500  FORMAT B
510  REM ATN IS RESET BY OUTPUT (13,500)512;
520  REM THESE COMMANDS MAY BE CONCATENATED TO GENERATE UNIVERSAL COMMANDS
530  OUTPUT (A1,500)256,1,512;
540  REM WILL SET ATN, OUTPUT A GO TO LOCAL CHARACTER 'GTL=01', THEN TURN ATN OFF
550  REM
560  OUTPUT (A1,500)768;
570  REM WILL ASSERT THE REN LINE TO ENABLE INSTRUMENTS IN THE REMOTE MODE
580  REM ****NOTE INSTRUMENT WILL NOT GO REMOTE UNTIL ADDRESSED. .
590  REM UNIT WILL STAY REMOTE UNTIL A 'GTL' OR REN IS RESET. .
600  REM  UNLISTEN ALL DEVICES
610  CMD "?"
620  REM REN IS RESET BY;
630  OUTPUT (A1,500)1024;
640  DISP "END TEST";
650  STOP
660  REM
670  REM ************************************************************************************
680  REM
690  REM  SAMPLE PROGRAM
700  A=0
710  F=123456
720  O=M=U=0
730  REM MODE=FUNCTION=0=CONTINUOUS, SIN WAVE. . .
740  REM ADDRESSES THE UNIT ON THE H-P INTERFACE BUS WITH REN ENABLED
750  OUTPUT (13,500)768
760  CMD "?U>"
770  OUTPUT (13,780)A,F,O,U,M;
780  FORMAT "G1A",E9.2,"F",E9.2,"D",F6.2,"B",F4.0,"C",F4.0,"HA"
790  REM LAST A DISPLAYS AMPLITUDE ON MODEL 159 DISPLAY. . .
800  FOR L=1 TO 100
810  OUTPUT (13,820)A;
820  FORMAT "A",E1000.2
830  A=9.99*RND(5)
840  DISP L
850  NEXT L
860  REM SENDS GTL TO ADDRESSED UNIT ONLY TO ENABLE KEYBOARD. . .
```

```
870   OUTPUT (13,500)256,1,512;
880   REM REN IS STILL ASSERTED.
890   DISP "STOP ** CONT-EXE TO REPEAT";
900   CMD "?"
910   STOP
920   GOTO 700
930   REM NOTE STOP BUTTON WILL ISSUE EOP-ICL INTRFC CLEAR WHICH WILL SEND
940   REM 159 TO LOCAL MODE. . . .
950   REM
960   REM ************************************************************************************
970   REM
980   END
```

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	ECN 1368	RO	11-11-75	

A3 ANALOG BD
1100-00-0107

A5 - DISPLAY BOARD
0103-00-0105

A6 - KEY BOARD
0103-00-0109

A2 DIGITAL BD
1100-00-0106

A4 IEC INTERFACE
1100-00-0145

A1 POWER SUPPLY BD
1100-00-0108

NOTE: UNLESS OTHERWISE SPECIFIED

NOTES
1. ▭ DENOTES ACTUAL LABELING ON UNIT
2. BAR OVER MNEMONIC DENOTES TRUE WHEN LOW
3. ○ DENOTES WIRE COLOR PER RESISTOR CODE

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN BARNETT	DATE 6/6	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR KP Schmidt	11/21/74	TITLE INTERCONNECT DIAGRAM IEC INTERFACE OPTION
FINISH WAVETEK PROCESS	RELEASE APPROV [illegible]	11/21/74	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1 .XX ±.030
	DO NOT SCALE DWG		MODEL NO 158-5
	SCALE		DWG NO 0004-00-0030 REV A
			CODE IDENT 23338 SHEET / OF /

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP
A	REMOVED C13, C17 + C20	RD	4/8/81	

C14, C15, C16, C18 AND C26 THRU C30 ARE .1/50V

C25 1000/35V

L58

GND B THIS AREA

MSB

1. ☐ DENOTES ACTUAL LABELING ON BOARD
1. * DENOTES OPEN COLLECTOR. NOTE UNLESS OTHERWISE SPECIFIED
2. X-XX REFERS TO PIN AND IC NUMBERS FOR IN-LINE RESISTOR PACS.
3. BAR OVER MNEMONIC DENOTES: TRUE-WHEN-LOW.

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN S.CHERMACK	DATE 7-30-81	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL —	PROJ ENGR		TITLE: SCHEMATIC, IEC INTERFACE
FINISH WAVETEK PROCESS —	RELEASE APPROV		
	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ± .010 ANGLES ± 1 XX ± .030		MODEL NO 158
	DO NOT SCALE DWG		DWG NO 0103-00-0972 REV B
	SCALE —		CODE IDENT 23338 SHEET 1 OF 1

B 3790 (Cl II) 5-27-83

BISHOP GRAPHICS/ACCUPRESS RECORDER NO. A-3894

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

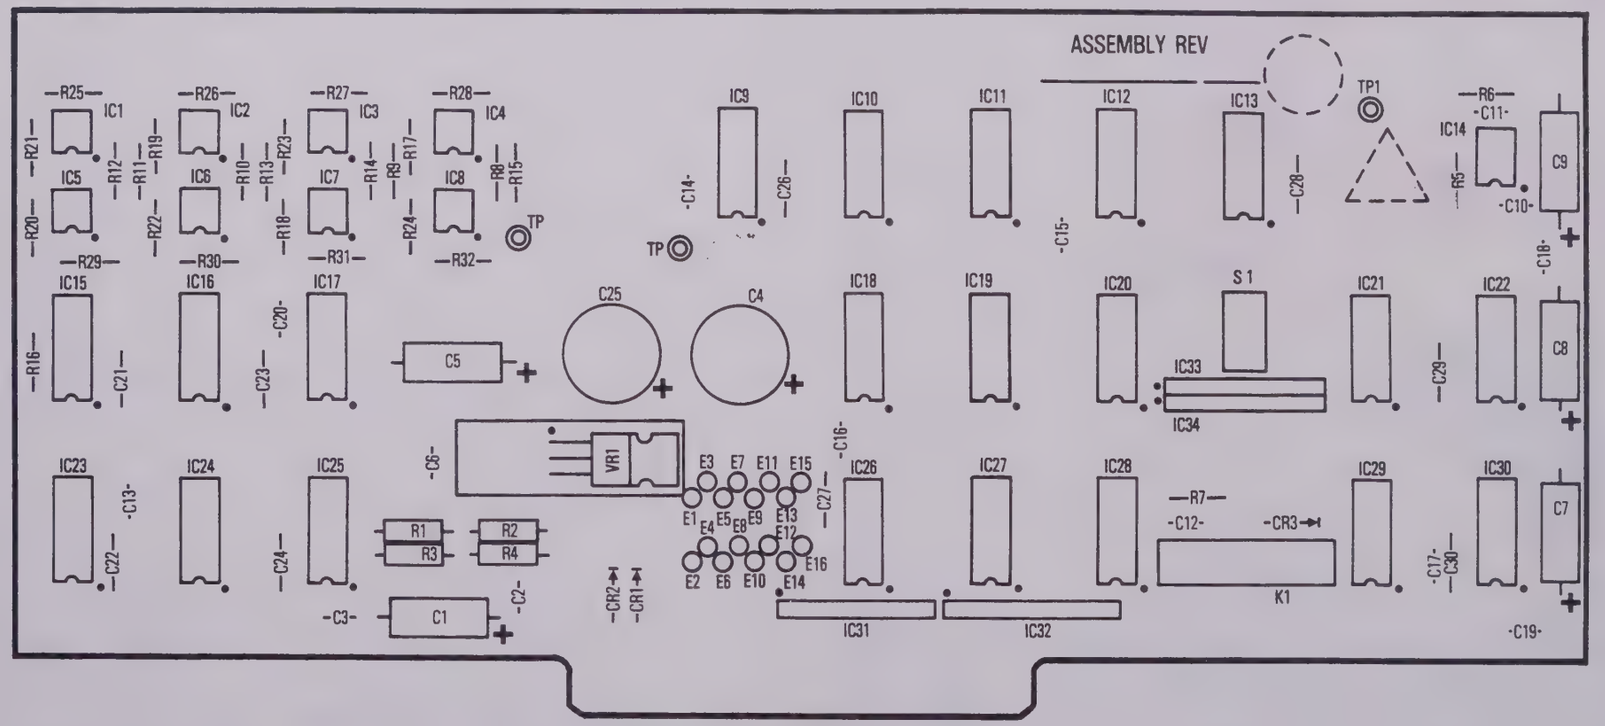

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: PCA GPIB INTERFACE BD. OPT. 005
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ±.010 ANGLES ±1 XX ±.030		MODEL NO 159 / DWG NO 0101-00-0972 / REV
	DO NOT SCALE DWG		CODE IDENT 23338 / SHEET OF
	SCALE		

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	ASSY DRWG, IEC INTERFACE	0101-00-0972	WVTK	0101-00-0972	1
NONE	SCHEMATIC, IEC INTERFACE	0103-00-0972	WVTK	0103-00-0972	1
C11	CAP, CER, MN, .01MF, 50V	CAC02Z5U103Z100A	CORNG	1500-01-0310	1
C12 C14 C15 C16 C18 C2 C21 C22 C23 C24 C26 C27 C28 C29 C30 C6	CAP, CER, MON, .1MF, 50V	CAC03Z5U104Z050A	CORNG	1500-01-0405	16
C10	CAP, CER, 470PF, 1KV	DD-471	CRL	1500-04-7111	1
C25 C4	CAP, ELECT, 1000MF/35V RADIAL LEAD, SP .30	CRE-SERIES-1000/35	CAPAR	1500-31-0202	2
C19	CAP, TANT, 22MF, 15V	196D226X9015KA1	SPRAG	1500-72-2601	1
C3	CAP, TANT, 27MF, 35V	196D276X0035TE4	SPRAG	1500-72-7602	1
C1 C5 C7 C8 C9	CAP, TANT, 33MF, 10V	1[illegible]D336X9010B2	SPRAG	1500-73-3601	5
NONE	IEC INTERFACE	1700-00-0972	WVTK	1700-00-0972	1
NONE	PIN, MALE	61182-2	AMP	2100-05-0020	3
NONE	STANDOFF, SWAGE .125 H, .250 DIA 4-40, .062 MAT'L	9531B-0440-3A	AMTOM	2800-03-0004	2
NONE	HEAT SINK	2800-11-0002	WVTK	2800-11-0002	1
NONE	WASHER, SHOULDER	2661	SMITH	2800-27-0002	2

WAVETEK PARTS LIST | TITLE: PCA, IEC INTERFACE | ASSEMBLY NO. 1100-00-0972 | PAGE: 1 | REV

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
K1	RELAY, REED, FORM-A	RA3019-1051	ETROL	4500-00-0007	1
R1 R2 R3 R4	RES, C, 1/2W, 5%, 10	RC20GF-100	STKPL	4700-25-0100	4
R10 R11 R12 R13 R14 R15 R8 R9	RES, MF, 1/8W, 1%, 150	RN55D-1500F	TRW	4701-03-1500	8
R17 R18 R19 R20 R21 R22 R23 R24	RES, MF, 1/8W, 1%, 20.5K	RN55D-2052F	TRW	4701-03-2052	8
R16	RES, MF, 1/8W, 1%, 2.21K	RN55D-2211F	TRW	4701-03-2211	1
R6	RES, MF, 1/8W, 1%, 30.1K	RN55D-3012F	TRW	4701-03-3012	1
R5	RES, MF, 1/8W, 1%, 4.99K	RN55D-4991F	TRW	4701-03-4991	1
R7	RES, MF, 1/8W, 1%, 61.9	RN55D-61R9F	TRW	4701-03-6199	1
R25 R26 R27 R28 R29 R30 R31 R32	RES, MF, 1/8W, 1%, 78.7K	RN55D-7872F	TRW	4701-03-7872	8
IC31 IC32 IC33 IC34	RESISTOR MOD	159-520	WVTK	4770-00-0005	4
CR1 CR2	DIODE	1N4002	FAIR	4801-02-0001	2
CR3	DIODE	1N4148	FAIR	4807-02-6666	1
S1	SWITCH PC	500-105	DUNCN	5199-00-0001	1
IC1 IC2 IC3 IC4 IC5 IC6 IC7 IC8	OPTO-COUPLER	4N26	MOT	7000-04-2600	8
IC14	IC	NE555V	SIG	7000-05-5500	1

WAVETEK PARTS LIST | TITLE: PCA, IEC INTERFACE | ASSEMBLY NO. 1100-00-0972 | PAGE: 2 | REV

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
IC19 IC23 IC24	IC	7400	TI	8000-74-0000	3
IC26 IC27	IC	7404	TI	8000-74-0400	2
IC18 IC20	IC	7405	TI	8000-74-0500	2
IC30	IC	7408	TI	8000-74-0800	1
IC21	IC	7410	TI	8000-74-1000	1
IC11	IC	7430	TI	8000-74-3000	1
IC10 IC17 IC25 IC29 IC9	IC	7438	TI	8000-74-3800	5
IC28	IC	7474	TI	8000-74-7400	1
VR1	VOLTAGE REGULATOR	MA7805UC	FAIR	8000-78-0500	1
IC12 IC13	IC	8242	SIG	8000-82-4200	2
IC22	IC	74107	TI	8007-41-0700	1
IC15 IC16	IC	74132	TI	8007-41-3200	2

WAVETEK PARTS LIST | TITLE: PCA, IEC INTERFACE | ASSEMBLY NO. 1100-00-0972 | PAGE: 3 | REV

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO, CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: PARTS LIST PCA, IEC INTERFACE
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ± .010 ANGLES ±1 XX ± .030		
	DO NOT SCALE DWG		MODEL NO 159 / DWG NO 1100-00-0972 / REV
	SCALE		CODE IDENT 23338 / SHEET 1 OF 1

B-SHOP GRAPHICS/ACCUPRESS REORDER NO. A-3884

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

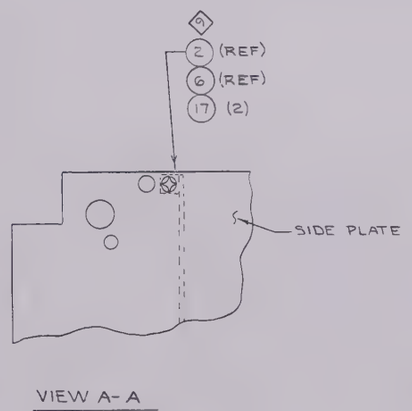

VIEW A-A

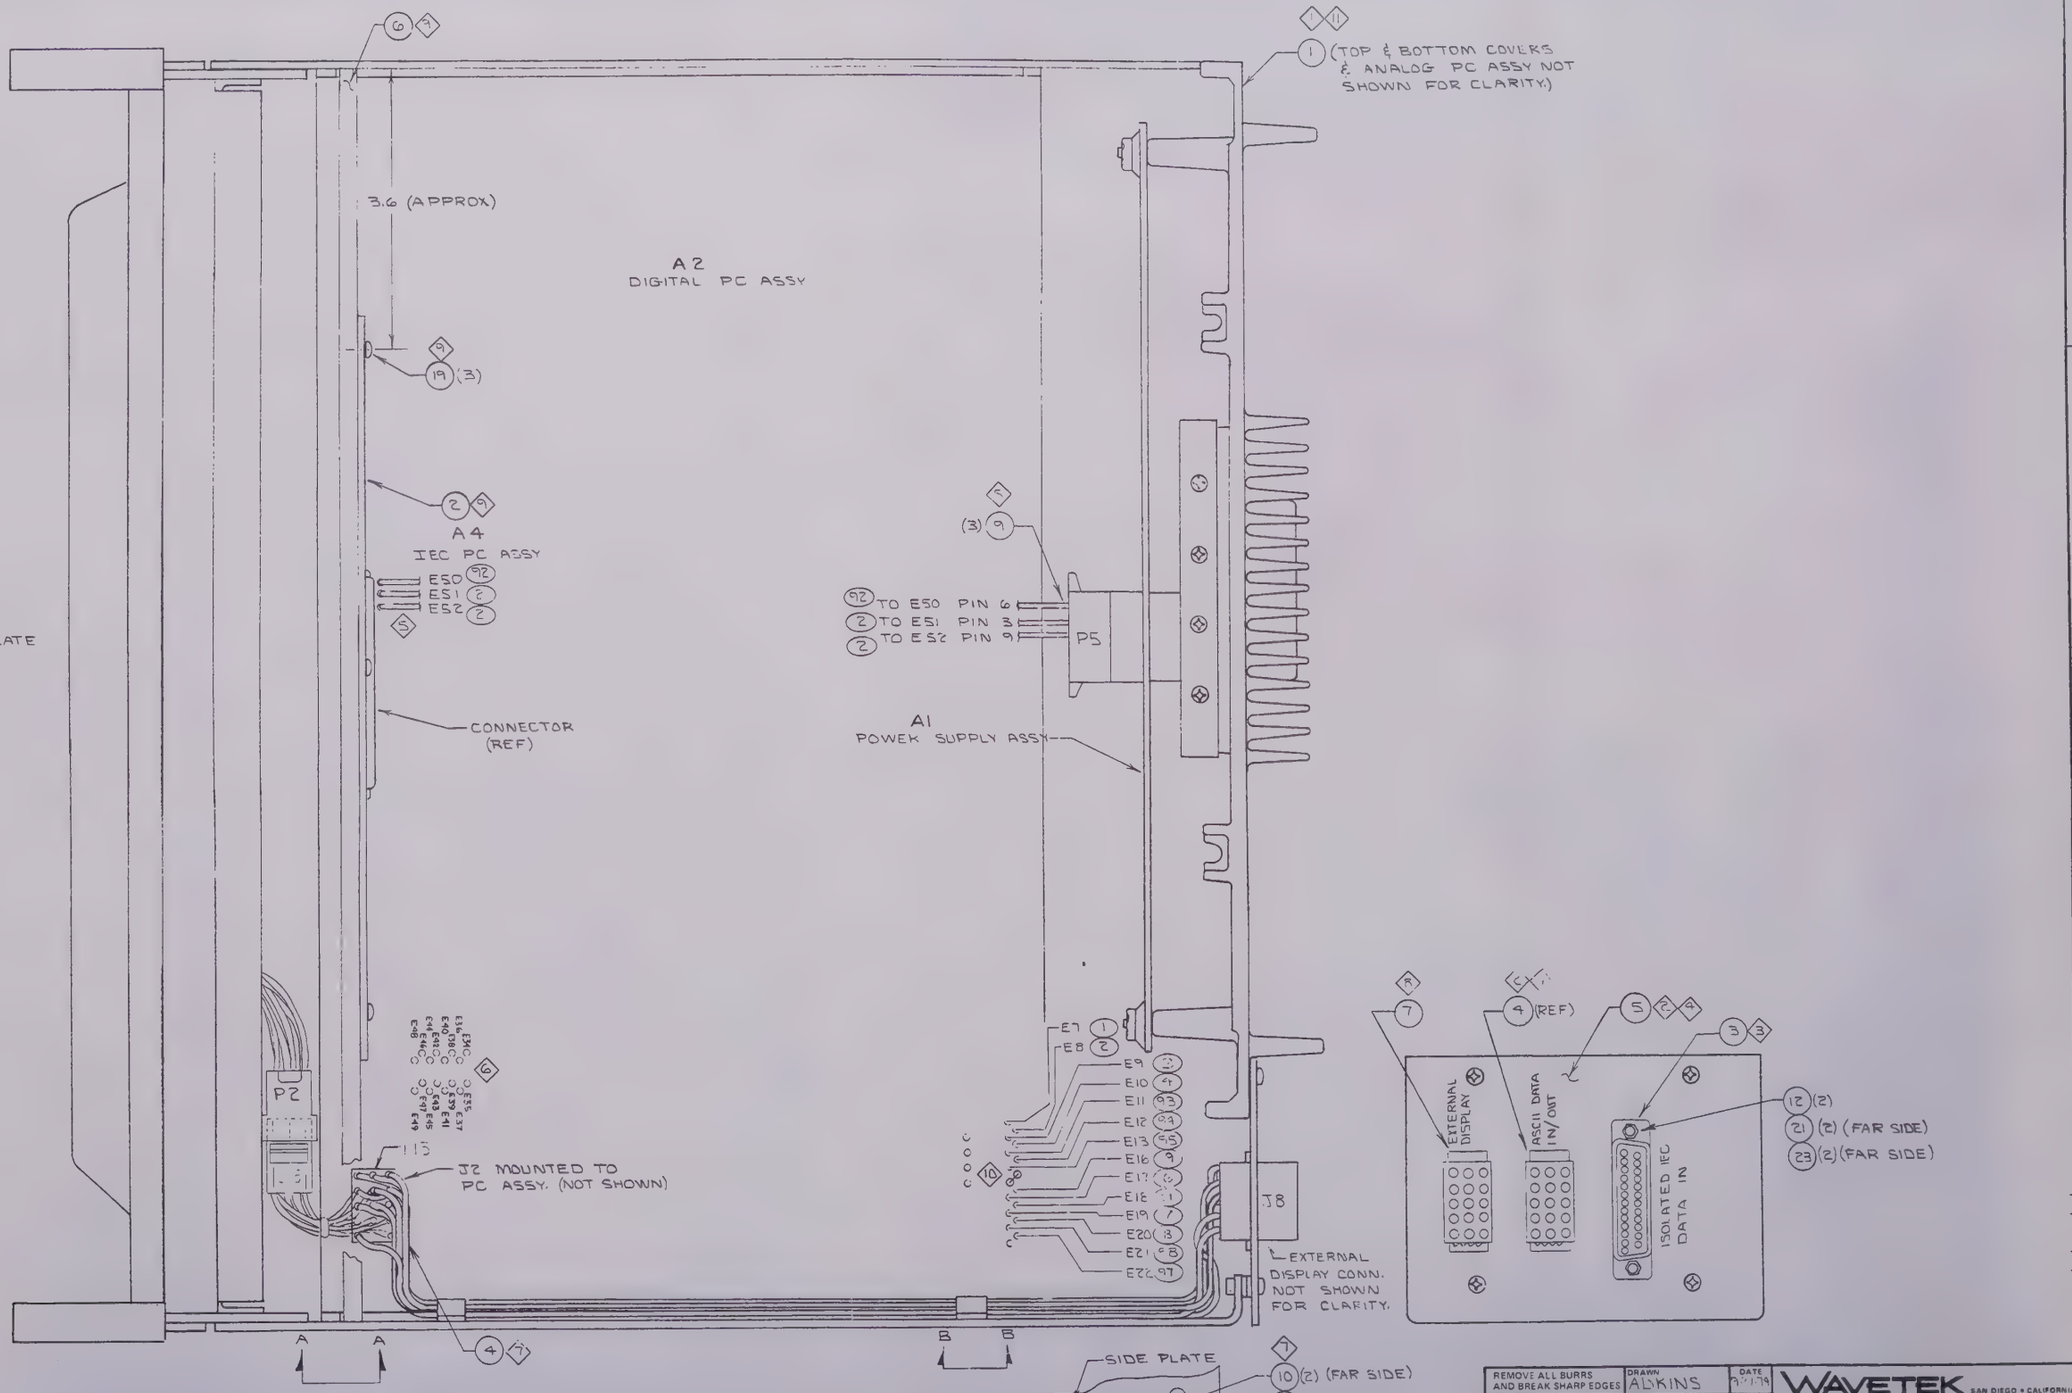

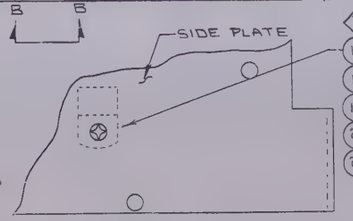

VIEW B-B

4. PULL HARDWARE FOR FIELD INSTALLATION ONLY.
3. ◇ DENOTES LINE NUMBER FOR MODIFICATION PROCEDURE. (SEE SHT 2.)
2. PROGRAMING MATING CONNECTORS: IDENTIFY PARTS BY BAG AND TAG AND SHIP WITH INSTRUMENT.
1. ○ DENOTES WIRE COLOR PER RESISTOR CODE.

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN ALKINS	DATE 9/1/79	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PRO. ENGR LPS Schwenck	10/21/79	TITLE MODIFICATION DWG IEC OPTION
	RELEASE APPROV LPS	10/24/79	
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ± .010 ANGLES ±1 XX ± .030		
	DO NOT SCALE DWG	MODEL NO 159	DWG NO 0102-00-0351 REV
	SCALE 1/1	CODE IDENT 23338	SHEET 1 OF 2

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

MODIFICATION PROCEDURE
IEC OPTION

1. REMOVE TOP AND BOTTOM COVERS.
2. REMOVE ASCII DATA IN/OUT MOLEX CONNECTOR J9 FROM EXISTING REAR PANEL EXTENDER P/N1400-00-0710. REMOVE REAR PANEL EXTENDER AND RETURN TO STOCK. UN-SOLDER ALL WIRES THAT GO TO THE A2 DIGITAL PC ASSY, FROM ASCII DATA IN/OUT CONNECTOR J9, AND RETURN THE CONNECTOR ASSY TO STOCK.
3. INSTALL THE IEC CABLE ASSY, P/N1203-00-0002 AND CONNECT WIRES AS SHOWN (REF INTERCONNECT 158-230 J9)
4. INSTALL EXTENDER REAR CASTING P/N1400-00-5590 AS SHOWN.
5. DISCONNECT THE MOLEX CONNECTOR, P5, FROM THE POWER SUPPLY PC ASSY A1. ATTACH MOLEX PINS P/N2100-05-0026, QTY (3), TO THE ENDS OF THREE WIRES. TWO OF THE WIRES TO BE, 22 AWG, RED, 13.5 INCHES LONG, AND ONE WIRE TO BE 22 AWG, WHT/RED, 13.5 INCHES LONG. INSTALL THE MOLEX PINS AND WIRES INTO P5 AS SHOWN AND SOLDER THE OTHER ENDS TO E50, E51, AND E52. (REF INTERCONNECT 158-.30 P5)
6. REMOVE JUMPERS FROM PADS E34 THRU E49 ON A2 DIGITAL PC ASSY.
7. DISCONNECT KEYBOARD MOLEX P2 FROM J2 AND INSTALL CONNECTOR ASSY, ASCII DATA IN/OUT, PN1203-00-0003 TO J2. CONNECT THE OTHER END TO THE KEYBOARD MOLEX P2. CONNECT THE OTHER END TO THE KEYBOARD MOLEX P2. INSTALL MOLEX J8, TO ASCII DATA IN/OUT, LOCATED ON THE REAR PANEL EXTENDER AS SHOWN.
8. INSTALL EMPTY MOLEX CONNECTOR P/N 2100-02-0012, IN THE EXTERNAL DISPLAY LOCATION ON THE EXTENDER REAR CASTING P/N 1400-00-5590.
9. INSTALL MTG BAR (OPTION CARD) P/N1400-00-5583, TO PC ASSY IEC, P/N1100-00-0142, AS SHOWN AND PLUG INTO CONNECTOR ON A2 DIGITAL PC BOARD.
   NOTE: IF PHOTO ISOLATION IS NOT REQUIRED INSTALL JUMPERS TO PADS E1 AND E2, E3 AND E4, E5 AND E6, E7 AND E8, E9 AND E10, E11 AND E12, E13 AND E14, E15 AND E16 AS SHOWN ON THE IEC PC ASSY.
10. INSTALL A JUMPER FROM E14 TO E15, ON THE A2 DIGITAL PC ASSY AS SHOWN.
11. INSTALL TOP AND BOTTOM COVERS.

SH2

DWG NO	REV
0102-00-0351	

SH3

DWG NO.	REV
0102-00-0351	

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE 8-10-79	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: MODIFICATION IEC OPTION
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED XXX ±.010 ANGLES ±1 XX ±.030		
	DO NOT SCALE DWG		MODEL NO. 159 / DWG NO. 0102-00-0351 / REV
	SCALE		CODE IDENT 23338 / SHEET 2 OF 2

BISHOP GRAPHICS/ACCUPRESS REORDER NO A-3994

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
NONE	ASSY DRWG, IEC MOD	0102-00-0351	WVTK	0102-00-0351	1
3	CABLE ASSY	158-033	WVTK	1207-00-0004	1
4	CABLE ASSY	158-035	WVTK	1207-00-0005	1
6	BAR, SUPT	158-330	WVTK	1400-00-5583	1
5	EXT, CASTING	158-333	WVTK	1400-00-5590	1
7	CONN, 15PIN	03-09-1151	MOLEX	2100-02-0012	1
8	PLUG, 15PIN	03-09-2151	MOLEX	2100-02-0013	1
NONE	PIN, MALE	02-09-2118	MOLEX	2100-03-0005	18
10	CABLE CLAMP	835	SMITH	2800-00-0010	2
11 11A	RETAINER, SPRING	D-191	WEKSR	2800-09-0007	2
12 12A	JACK SCREW	408-146475	AMPH	2800-23-0008	2

WAVETEK PARTS LIST	TITLE MODIFICATION KIT	ASSEMBLY NO. 1101-00-0229 PAGE: 1	REV B

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE: PARTS LIST MODIFICATION KIT
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1 .XX ±.030		
	DO NOT SCALE DWG	MODEL NO 159	DWG NO 1101-00-0229 REV B
	SCALE	CODE IDENT 23338	SHEET 1 OF 1

BISHOP GRAPHICS/ACCUPRESS REORDER NO. A-3894

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

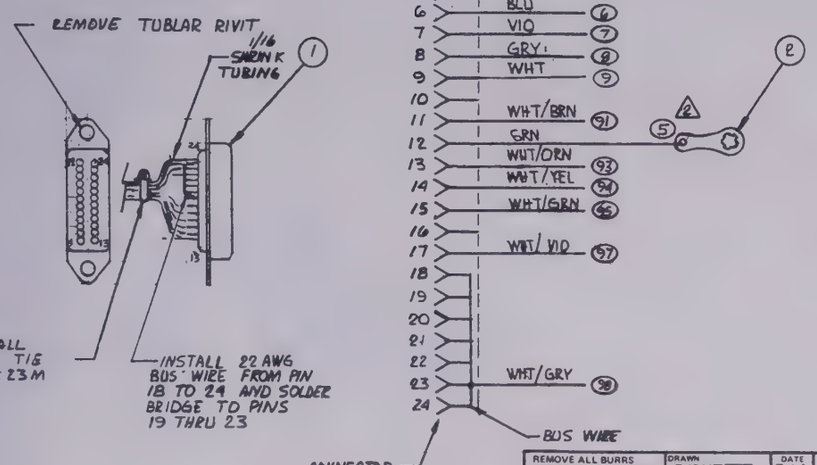

4. SOLDER WIRES TO CONNECTOR AS SHOWN IN DIAGRAM.
3. CUT WIRES TO A LENGTH OF 5.00.
△2 CUT WIRE TO A LENGTH OF 3.50 AND SOLDER TO LUG
1. ○ DENOTES WIRE COLOR PER RESISTOR COLOR CODE

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN BARNETT	DATE 7-24	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE CABLE ASSY- IEC OPTION
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030		
	DO NOT SCALE DWG		MODEL NO 159-005 / DWG NO. 1203-00-0002 / REV
	SCALE FULL		CODE IDENT 23338 / SHEET 2 OF 2

REFERENCE DESIGNATORS	PART DESCRIPTION	ORIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
1	CONN	57-20240	AMPH	2100-02-0060	1
2	TERM,LOCK LUG	1414-6	SMITH	2100-04-0009	1

WAVETEK PARTS LIST	TITLE CABLE ASSY	ASSEMBLY NO. 1207-00-0004 PAGE: 1	REV

© 1983 WAVETEK, INC. ALL RIGHTS RESERVED. PRINTED IN U.S.A.

NOTE UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN	DATE	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	PROJ ENGR		TITLE CABLE ASSY IEC (GPIB) OPTION
	RELEASE APPROV		
FINISH WAVETEK PROCESS	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030		
	DO NOT SCALE DWG		MODEL NO. 159-005 / DWG NO. 1207-00-0004 / REV
	SCALE		CODE IDENT 23338 / SHEET 1 OF 1

© BISHOP GRAPHICS/ACCUPRESS REORDER NO. A-8884

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND DESIGN RIGHTS BELONGING TO WAVETEK AND MAY NOT BE REPRODUCED FOR ANY REASON EXCEPT CALIBRATION, OPERATION, AND MAINTENANCE WITHOUT WRITTEN AUTHORIZATION.

REV	ECN	BY	DATE	APP

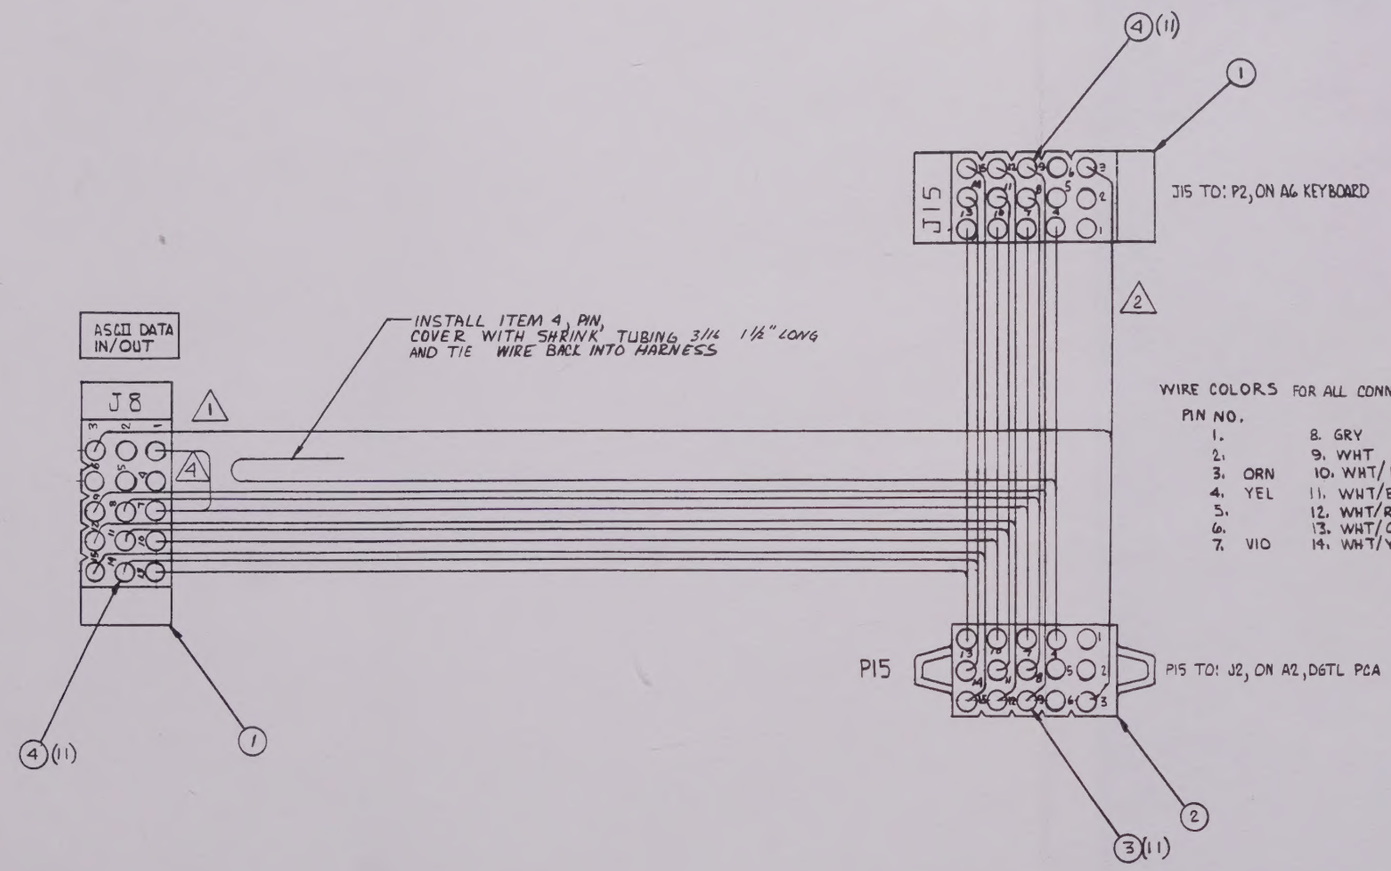

WIRE COLORS FOR ALL CONNECTORS

PIN NO.			
1.		8. GRY	15. WHT/GRN
2.		9. WHT	
3.	ORN	10. WHT/BLK	
4.	YEL	11. WHT/BRN	
5.		12. WHT/RED	
6.		13. WHT/ORN	
7.	VIO	14. WHT/YEL	

REFERENCE DESIGNATORS	PART DESCRIPTION	OMIG-MFGR-PART-NO	MFGR	WAVETEK NO.	QTY/PT
1 1A	CONN, 15PIN	03-09-1151	MOLEX	2100-02-0012	2
2	PLUG, 15PIN	03-09-2151	MOLEX	2100-02-0013	1
NONE	PIN, MALE	02-09-2110	MOLEX	2100-03-0005	11
NONE	PIN, FEMALE	02-09-1110	MOLEX	2100-03-0002	22

WAVETEK PARTS LIST	TITLE CABLE ASSY	ASSEMBLY NO. 1207-00-0005 PAGE: 1	REV

4. WIRE COLOR TO BE VIO CUT WIRE TO A LENGTH OF 1.00
3. TIE WIRES USING SMALL CABLE TYE 23M AS REQ.
2. CUT WIRES TO A LENGTH OF 3.00
1. CUT WIRES TO A LENGTH OF 16.50

NOTE: UNLESS OTHERWISE SPECIFIED

REMOVE ALL BURRS AND BREAK SHARP EDGES	DRAWN BARNETT	DATE 8/6/84	WAVETEK SAN DIEGO • CALIFORNIA
MATERIAL	ENGINEER	8/10/84	TITLE CONNECTOR ASSY ASCII DATA IN/OUT
FINISH WAVETEK PROCESS	RELEASE APPROV	12/4/84	
	TOLERANCE UNLESS OTHERWISE SPECIFIED .XXX ±.010 ANGLES ±1° .XX ±.030		
	DO NOT SCALE DWG		MODEL NO. 158/159 DWG NO. 1203-00-0003 REV
	SCALE NONE		CODE IDENT 23338 SHEET 2 OF 2

www.manualsplus.com
1030117